BMC Branan Medical Corporation

The Fastect® II Drug Screen Dipstick Test is a simple one-step dipstick device for the rapid qualitative detection of drugs of abuse in human urine.

Fastect® II Procedures -- Refer to package insert for detailed instructions and technical information.

1. **Remove** the Fastect® II test device from the sealed pouch and **slide** the protective sleeve all the way up.

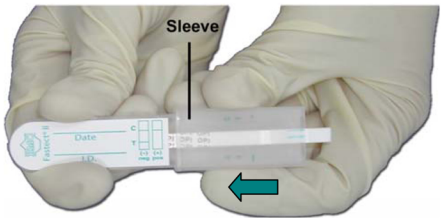

2. Dip the sample pad of the test device into the urine specimen to the maximum dip level for at least 10 seconds. **Dip up to and not beyond the tips of the arrows.**

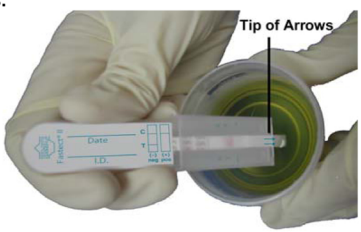

3. **Slide** the sleeve down to the **read indicator mark** and lay the device on a level surface.

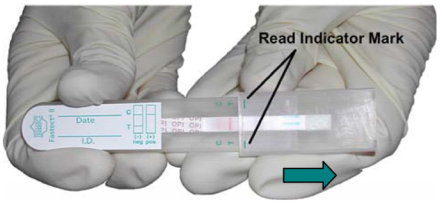

4. **Read** the results once the **control band (C)** appears (in approximately 5 minutes). Results may be interpreted up to 1 hour. Do not read after 1 hour.

Interpreting Fastect® II Test Results

Invalid Result

When **no** band appears in the **CONTROL (C) region**, **the test is invalid** even if there is a band in the test region. Check testing procedures, and samples. Repeat the test with a new device.

Example Interpretation:

THC: Invalid
COC: Invalid

Negative Result

For each test, two colored bands should be observed:

- **One in the CONTROL (C) region**
- **One in the specific TEST region**

The color of the test band may be slightly darker or lighter than the control band. Any band that can be seen visually is a **negative** result.

Example Interpretation:



THC: Negative
COC: Negative

Presumptive Positive Result

A colored band at the **CONTROL (C) region** should be observed. When there is no colored band at the specific **TEST region**, the test is presumptive positive for that particular drug.

Example Interpretation:

THC: Negative
COC: **Positve**