



friendly
technology



Smart monitoring
of warfarin therapy

microINR





**friendly
technology**

iLine Microsystems is a biotech company researching, developing and manufacturing POCT IVD devices in the Hemostasis area since 2007. The company incorporates proprietary technology that provides innovative and highly reliable products for the current and future needs of the changing healthcare models.





Microfluidic & Modular platform design

From a simple diagnostic solution to the modular platform concept to address coagulation diagnostic systems challenges.

iLine's Core Technology is based on microfluidic and Lab-on-a-Chip technology. This technology provides means to perform a biological test comprising sample application, reagent storage, mixing, detection and QC, all these embedded in a miniaturized chip using a minimum volume of blood sample. This innovative concept retains quality

equivalents to the classical laboratory processes, and it also provides the advantages of a user-friendly one-step assay. The Core Technology comprises means for Chip manufacturing, based in microengineering and microfabrication processes, which allows massive production that combines high quality at a significant cost efficiency.



microINR System

The microINR System is an in vitro diagnostics medical device, intended to monitor oral anticoagulation therapy (OAT) with warfarin.

The microINR System refers to the reader (microINR Meter) and the analytic test strips (microINR Chips). Our system provides quantitative determination of prothrombin

time (PT) in INR (International Normalized Ratio) units with fresh capillary blood performed by fingersticking.

The microINR System has been developed to fulfill the needs of all the existing OAT monitoring models and it is intended for patient self-testing use, as well as for healthcare professionals at

Point of Care settings.

The System employs patent granted technology, based on the iLine's Core Technology and provides accurate and reproducible results as proven in extensive and independent performance evaluations.

microINR



Meter description

Consisting of a Machine Vision System (MVS) that provides interfacing and detection means, the **microINR Meter** also offers the best qualities of a portable coagulometer:

no buttons to be pressed during the testing, automatic strip identification, minimum sample volume and easy-to-use design.

Meter dimensions

119 x 65 x 35 mm

Screen dimensions

45 x 45 mm

2 Buttons

For time/date settings and turning on/off

View data history

Up to 199 tests and error messages

Power supply:

Rechargeable battery (approx. 70 Test per battery cycle)


microINR Chips

Working principle

INR determination through sample flow monitoring along microcapillaries, following activation of the coagulation cascade. The current IVD test mimics the conditions of “in vivo” hemostasis, also referred as “ex vivo” (1).

Chip description

Disposable plastic test strip, that encloses two microcapillary channels, of extremely simple construction and fully passive (i.e. no built-in sensors, nor electrodes, nor external pumping).

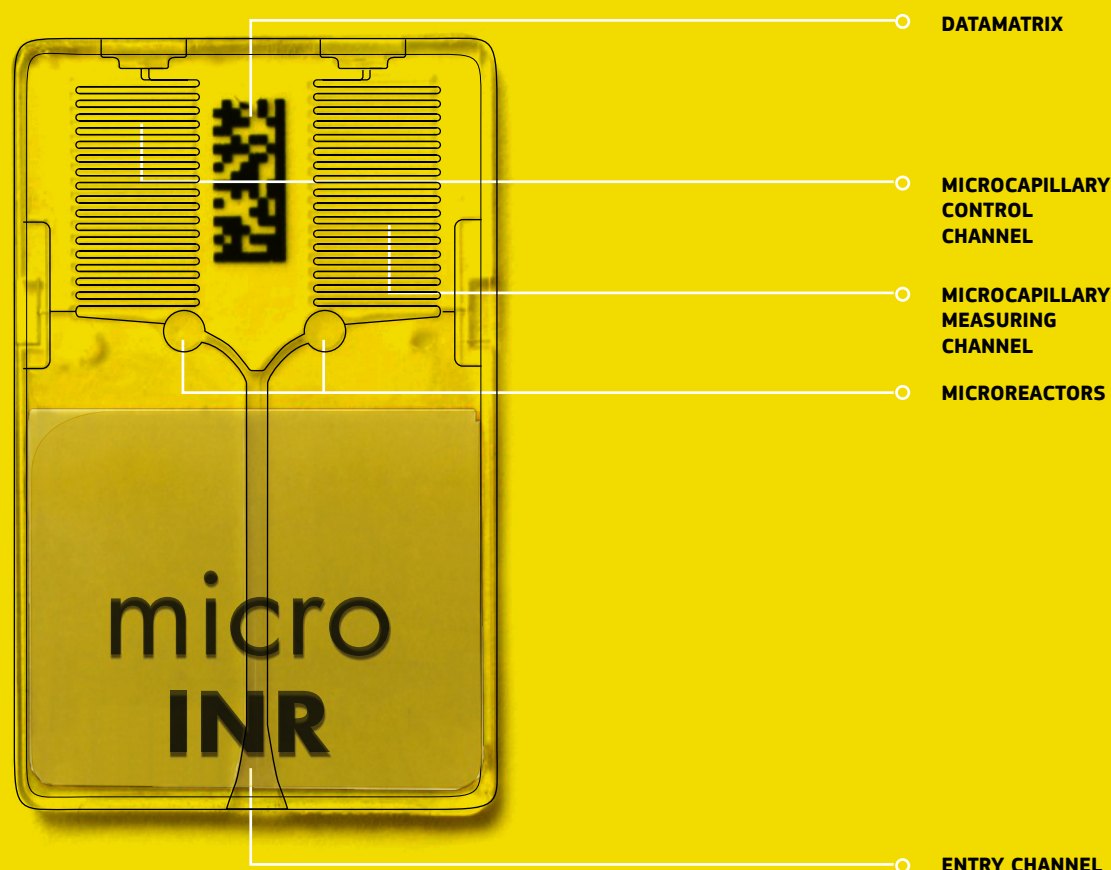

(1) Armando Tripodi, The history of Phenotypic testing in Thrombosis and Hemostasis, Seminars in Thrombosis and Hemostasis, 2008, Volume 34, number 7

Chip specifications

High sensitivity human recombinant thromboplastin

Chip expiry and calibration parameters coded and integrated into the Chip

Real control assay simultaneously at parallel channel

Individually packed

Storage at room temperature (36-77°F)

15 Months shelf life

System specifications

3 µL sample volume required

Measurement range: 0.8 - 4.5 INR

System ISI: Approx. 1

Integrated and independent on-board QC



microINR

User-friendly

No calibration chip needed

Fully automatic

Rapid test performance (less than 1 minute)

Easy-to-use: testing steps set to the minimum

Small sample volume

Painless fingersticking

Gentle fingersticking reduces forced tissue factor activation

Less prone to insufficient sample volume errors

Reliability

Enhanced multilevel QC strategy assesses all possible sources of error

Safety


Automatic lot ID: No calibration chip needed

Test results only reported in INR units

System protected for values above 4.5 INR

Step by step procedure

No buttons are needed to be pressed during this procedure. Test is fully completed in less than 1 minute. Acoustic signals and illumination of the Chip guide the user along key steps.

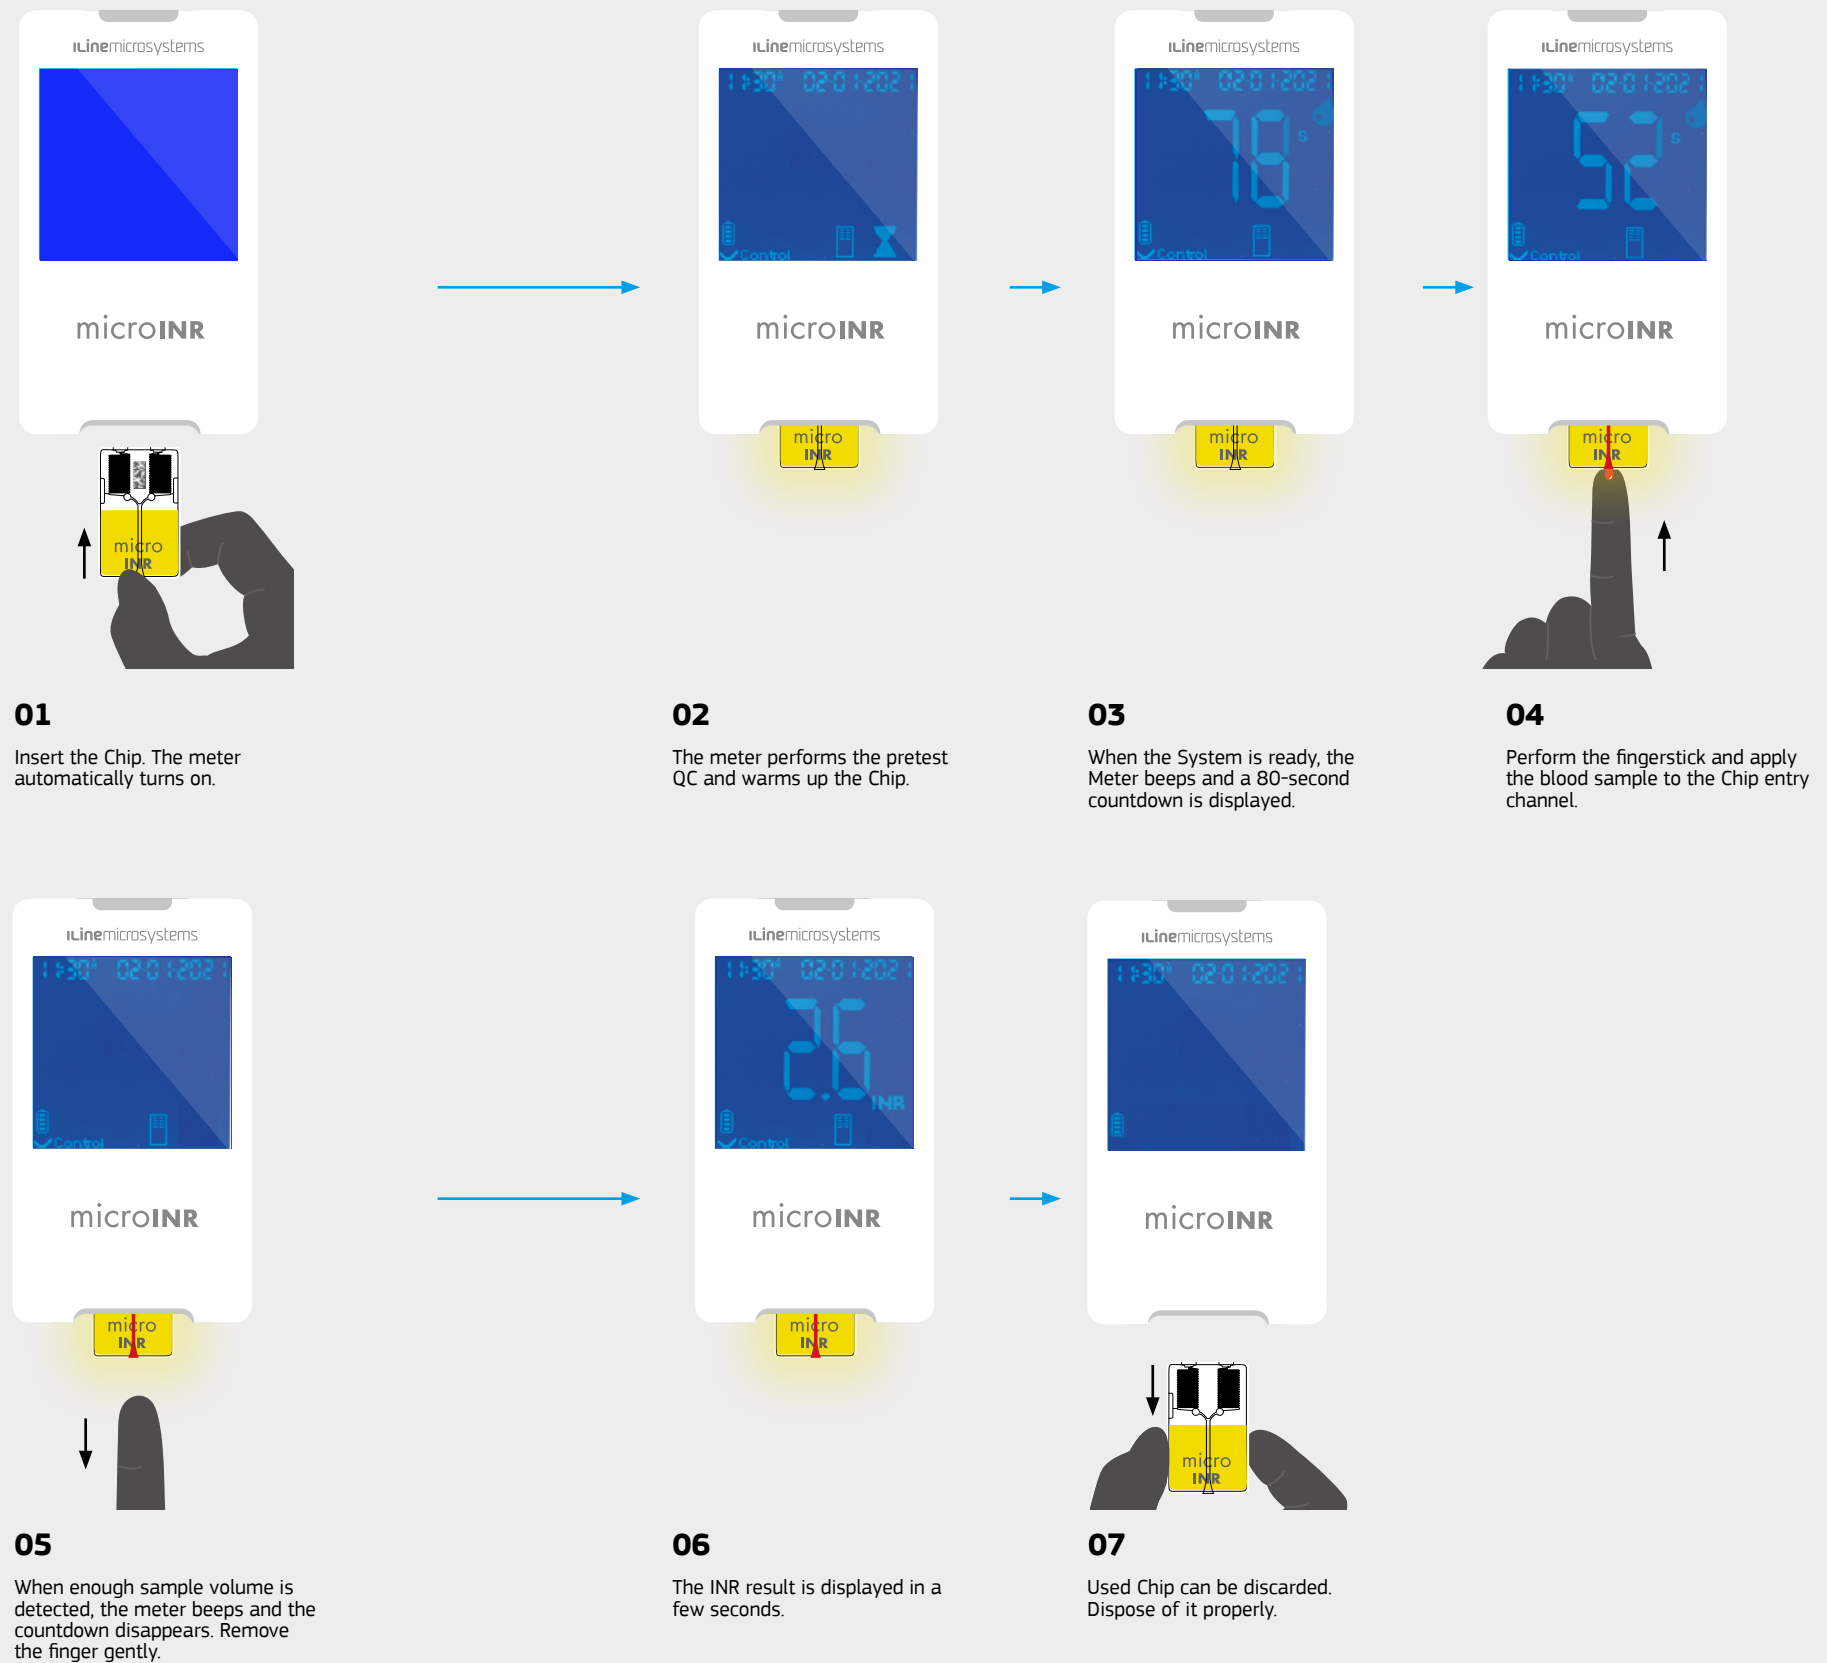

Our System

microINR METER



CASE



microINR CHIP



**friendly
technology**

CAT0001US - Rev. 2021-02

CLIA categorization

This System is for self-testing patients and for healthcare professionals at Point Of Care settings. This is a CLIA Waived test system. Facilities performing testing must have a CLIA Certificate of Waiver (or higher). Laboratories with a certificate of waiver must follow the manufacturer's instructions for performing a test. All applicable state and local laws must be met.

The information contained in this brochure is not applicable to all countries. Product registration and availability vary by country. For more information, please contact: info@ilinemicrosystems.com

iLine Microsystems S.L.
Paseo Mikeletegi 69
20009 Donostia (Gipuzkoa)
Spain

info@ilinemicrosystems.com
Tel. + 34 943 005 651
Fax. +34 943 008 737

www.ilinemicrosystems.com