



Mouse Albumin ELISA

For the measurement of albumin in serum, plasma or urine of mice.

Please see Appendix A for Reference Serum information.

For Research Use Only. Not For Use In Diagnostic Procedures.

Catalog Number: 41-ALBMS-E01

Size: 96 wells

Version: V3 L61-51-ALPCO September 7, 2018

INTENDED USE

The Mouse Albumin ELISA is a highly sensitive two-site enzyme-linked immunoassay (ELISA) for measuring albumin in serum, plasma or urine of mice. For Research Use Only.

INTRODUCTION

Albumin is a polyfunctional protein contributing to homeostasis through mechanisms of hemodynamics, transport and nutrition. Albumin is found both intra- and extravascularly in all mammals and many lower vertebrates. It is a molecule of about 67,000 daltons, synthesized by the liver. Normally only very trace amounts of albumin escape reabsorption by kidney glomeruli and are excreted into the urine. Many occult diseases can cause kidney damage which may result in excessive amounts of serum proteins, including albumin, to be excreted by the kidney and into the urine. This ELISA kit can be used to measure albumin in serum, plasma, or urine of mice.

PRINCIPLE OF THE ASSAY

The principle of the double antibody sandwich ELISA is represented in Figure 1. In this assay, the Albumin present in samples reacts with the anti-Albumin antibodies which have been adsorbed to the surface of polystyrene microtiter wells. After the removal of unbound proteins by washing, anti-Albumin antibodies conjugated with horseradish peroxidase (HRP), are added. These enzyme-labeled antibodies form complexes with the previously bound Albumin. Following another washing step, the enzyme bound to the immunosorbent is assayed by the addition of a chromogenic substrate, 3,3',5,5'-tetramethylbenzidine (TMB). The quantity of bound enzyme varies directly with the concentration of Albumin in the sample tested; thus, the absorbance, at 450 nm, is a measure of the concentration of Albumin in the test sample. The quantity of Albumin in the test sample can be interpolated from the standard curve constructed from the standards and corrected for sample dilution.

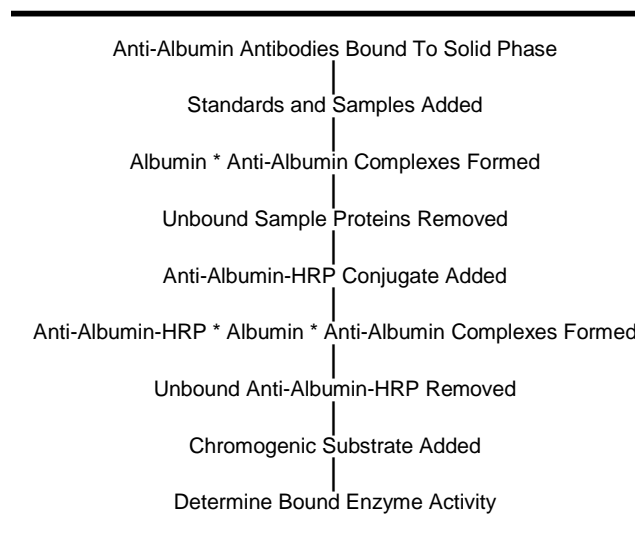


Figure 1.

REAGENTS (Quantities sufficient for 96 determinations)

1. **DILUENT CONCENTRATE (Assay Buffer)**
One bottle containing 50 mL of a 5X concentrated diluent assay buffer.
2. **WASH SOLUTION CONCENTRATE**
One bottle containing 50 mL of a 20X concentrated wash solution.

3. ENZYME-ANTIBODY CONJUGATE 100X
One vial containing 150 μ L of affinity purified anti-Mouse Albumin antibody conjugated with horseradish peroxidase in a stabilizing buffer.
4. CHROMOGEN-SUBSTRATE SOLUTION
One vial containing 12 mL of 3,3',5,5'-tetramethylbenzidine (TMB) and hydrogen peroxide in citric acid buffer at pH 3.3.
5. STOP SOLUTION
One vial containing 12 mL 0.3 M sulfuric acid.
WARNING: Avoid contact with skin.
6. ANTI-MOUSE ALBUMIN ELISA MICROPLATE
Twelve removable eight (8) well microwell strips in well holder frame. Each well is coated with affinity purified anti-Mouse albumin.
7. MOUSE ALBUMIN CALIBRATOR
One vial containing a lyophilized Mouse Albumin calibrator.

FOR RESEARCH USE ONLY

REAGENT PREPARATION

1. DILUENT CONCENTRATE
The Diluent Solution supplied is a 5X Concentrate and must be diluted 1:5 with distilled or deionized water (1 part buffer concentrate, 4 parts dH₂O).
2. WASH SOLUTION CONCENTRATE
The Wash Solution supplied is a 20X Concentrate and must be diluted 1:20 with distilled or deionized water (1 part buffer concentrate, 19 parts dH₂O). Crystal formation in the concentrate is not uncommon when storage temperatures are low. Warming of the concentrate to 30-35°C before dilution can dissolve crystals.
3. ENZYME-ANTIBODY CONJUGATE
Calculate the required amount of working conjugate solution for each microtiter plate test strip by adding 10 μ L Enzyme-Antibody Conjugate to 990 μ L of 1X Diluent for each test strip to be used for testing. Mix uniformly, but gently. Avoid foaming.
4. CHROMOGEN-SUBSTRATE SOLUTION
Ready to use as supplied.
5. STOP SOLUTION
Ready to use as supplied.
6. ANTI-MOUSE ALBUMIN ELISA MICROPLATE
Ready to use as supplied. Unseal Microtiter Pouch and remove plate from pouch. Remove all strips and wells that will not be used in the assay and place back in pouch with desiccant and re-seal.
7. MOUSE ALBUMIN CALIBRATOR
Add 1.0 mL of distilled or deionized water to the Mouse Albumin calibrator and mix gently until dissolved. The calibrator is now at a concentration of 42.75 μ g/mL (**the reconstituted calibrator should be aliquoted and frozen if future use is intended**). **Mouse Albumin standards need to be prepared immediately prior to use (see chart below)**. Mix well between each step. Avoid foaming.

Standard	ng/mL	Volume added to 1x Diluent	Volume of 1x Diluent
7	500	10 µL of Albumin Calibrator	845 µL
6	250	300 µL Standard 7	300 µL
5	125	300 µL Standard 6	300 µL
4	62.50	300 µL Standard 5	300 µL
3	31.25	300 µL Standard 4	300 µL
2	15.63	300 µL Standard 3	300 µL
1	7.81	300 µL Standard 2	300 µL
0	0		600 µL

STORAGE AND STABILITY

The expiration date for the package is stated on the box label.

1. DILUENT

The 5X Diluent Concentrate is stable until the expiration date. The 1X working solution is stable for at least one week from the date of preparation. Both solutions should be stored at 4-8°C.

2. WASH SOLUTION

The 20X Wash Solution Concentrate is stable until the expiration date. The 1X working solution is stable for at least one week from the date of preparation. Both solutions can be stored at room temperature (16-25°C) or at 4-8°C.

3. ENZYME-ANTIBODY CONJUGATE

Undiluted horseradish peroxidase anti-Albumin conjugate should be stored at 4-8°C and **diluted immediately prior to use**. The working conjugate solution is stable for up to 1 hour when stored in the dark.

4. CHROMOGEN-SUBSTRATE SOLUTION

The Substrate Solution should be stored at 4-8°C and is stable until the expiration date.

5. STOP SOLUTION

The Stop Solution should be stored at 4-8°C and is stable until the expiration date.

6. ANTI-MOUSE ALBUMIN ELISA MICROPLATE

Anti-Mouse Albumin coated wells are stable until the expiration date and should be stored at 4-8°C in sealed foil pouch with desiccant pack.

7. MOUSE ALBUMIN CALIBRATOR

The lyophilized Mouse Albumin calibrator should be stored at 4°C or frozen until reconstituted. The reconstituted calibrator should be aliquoted and stored frozen (avoid multiple freeze-thaw cycles). The working standard solutions should be prepared immediately prior to use.

INDICATIONS OF INSTABILITY

If the test is performing correctly, the results observed with the standard solutions should be within 20% of the expected values.

SAMPLE COLLECTION AND HANDLING

Blood should be collected by venipuncture. The serum should be separated from the cells after clot formation by centrifugation. For plasma samples, blood should be collected into a container with an anticoagulant and then centrifuged. Care should be taken to minimize hemolysis, as excessive hemolysis can impact the results. Assay immediately or aliquot and store samples at -20°C. Avoid repeated freeze-thaw cycles.

1. Precautions
For any sample that might contain pathogens, care must be taken to prevent contact with open wounds.
2. Additives and Preservatives
No additives or preservatives are necessary to maintain the integrity of the sample. Avoid azide contamination.
3. Known interfering substances
Azide and thimerosal at concentrations higher than 0.1% inhibit the enzyme reaction.

MATERIAL PROVIDED See "REAGENTS"

MATERIALS REQUIRED BUT NOT PROVIDED

- Precision pipette (2 µL to 1000µL) for making and dispensing dilutions
- Test tubes
- Microtiter washer/aspirator
- Distilled or Deionized H₂O
- Microtiter Plate reader
- Assorted glassware for the preparation of reagents and buffer solutions
- Timer
- Centrifuge
- Anticoagulant

ASSAY PROTOCOL

DILUTION OF SAMPLES

The assay for quantification of albumin in urine or serum requires that each test sample be diluted before use. A 1:500 dilution is appropriate for most urine samples while serum or plasma samples may need to be diluted 1:500,000. **For absolute quantification, samples that yield results outside the range of the standard curve, a lesser or greater dilution might be required.**

1. To prepare a 1:500 dilution of sample, transfer 2 µL of sample to 998 µL of 1X diluent. This gives a 1:500 dilution.
2. To prepare a 1:500,000 dilution, transfer 2 uL of sample to 1998 uL of 1X diluent. This gives a 1:1000 dilution. Then transfer 2 uL of the 1:1000 dilution to 998 uL of 1X diluent. This yields a 1:500,000 dilution.

PROCEDURE

1. **Bring all reagents to room temperature before use.**
2. Pipette 100 µL of:
Standard 0 (0.0 ng/mL) in duplicate
Standard 1 (7.81 ng/mL) in duplicate

Standard 2 (15.63 ng/mL) in duplicate
Standard 3 (31.25 ng/mL) in duplicate
Standard 4 (62.50 ng/mL) in duplicate
Standard 5 (125 ng/mL) in duplicate
Standard 6 (250 ng/mL) in duplicate
Standard 7 (500 ng/mL) in duplicate

3. Pipette 100 μ L of prepared sample (in duplicate) into pre-designated wells.
4. Incubate the microtiter plate at room temperature for thirty (30 ± 2) minutes. Keep plate covered and level during incubation.
5. Following incubation, aspirate the contents of the wells.
6. Completely fill each well with appropriately diluted Wash Solution and aspirate. Repeat three times, for a total of four washes. If washing manually: completely fill wells with wash buffer, invert the plate then pour/shake out the contents in a waste container. Follow this by sharply striking the wells on absorbent paper to remove residual buffer. Repeat 3 times for a total of four washes.
7. Pipette 100 μ L of appropriately diluted Enzyme-Antibody Conjugate to each well. Incubate at room temperature for thirty (30 ± 2) minutes. Keep plate covered in the dark and level during incubation.
8. Wash and blot the wells as described in Steps 5 and 6.
9. Pipette 100 μ L of TMB Substrate Solution into each well.
10. Incubate in the dark at room temperature for precisely ten (10) minutes.
11. After ten minutes, add 100 μ L of Stop Solution to each well.
12. Determine the absorbance (450 nm) of the contents of each well. Calibrate the plate reader to manufacturer's specifications.

STABILITY OF THE FINAL REACTION MIXTURE

The absorbance of the final reaction mixture can be measured up to 2 hours after the addition of the Stop Solution. However, good laboratory practice dictates that the measurement be made as soon as possible.

RESULTS

1. Subtract the average background value from the test values for each sample.
2. Using the results observed for the standards construct a Standard Curve. The appropriate curve fit is that of a four-parameter logistics curve. A second order polynomial (quadratic) or other curve fits may also be used.
3. Interpolate test sample values from standard curve. Correct for sera dilution factor to arrive at the Albumin concentration in original samples.

LIMITATION OF THE PROCEDURE

1. Reliable and reproducible results will be obtained when the assay procedure is carried out with a complete understanding of the information contained in the package insert instructions and with adherence to good laboratory practice.
2. Factors that might affect the performance of the assay include proper instrument function, cleanliness of glassware, quality of distilled or deionized water, accuracy of reagent and sample pipetting, washing technique, incubation time or temperature.
3. Do not mix or substitute reagents with those from other lots or sources.

Appendix A – Reference Serum Information

One vial containing a Reference Serum is included with this kit.
Please refer to the enclosed Product Profile Sheet for lot-specific information.
Please note the following:

1. The Reference Serum is stable until the expiry date.
2. The Reference Serum should be diluted as appropriate to fit within the standard curve range. Refer to the “Dilution of Samples” section of the protocol for instructions.
3. While pipetting the samples (Procedure section), also pipette the Reference Serum in duplicate.