

Galaxy Intrusion Integration for victor Unified Client

User Guide

Notice

The information in this manual was current when published. The manufacturer reserves the right to revise and improve its products. All specifications are therefore subject to change without notice.

Copyright

Under copyright laws, the contents of this manual may not be copied, photocopied, reproduced, translated or reduced to any electronic medium or machine-readable form, in whole or in part, without prior written consent of Tyco Security Products.

© 2021 Johnson Controls. All rights reserved. JOHNSON CONTROLS, TYCO and AMERICAN DYNAMICS are trademarks of Johnson Controls.

Customer Service

Thank you for using American Dynamics products. We support our products through an extensive worldwide network of dealers. The dealer through whom you originally purchased this product is your point of contact if you need service or support. Our dealers are empowered to provide the very best in customer service and support. Dealers should contact American Dynamics at (800) 507-6268 or (561) 912-6259 or on the Web at www.americandynamics.net.

Trademarks

Windows® is a registered trademark of Microsoft Corporation. PS/2® is a registered trademark of International Business Machines Corporation.

The trademarks, logos, and service marks displayed on this document are registered in the United States [or other countries]. Any misuse of the trademarks is strictly prohibited and Tyco Security Products will aggressively enforce its intellectual property rights to the fullest extent of the law, including pursuit of criminal prosecution wherever necessary. All trademarks not owned by Tyco Security Products are the property of their respective owners, and are used with permission or allowed under applicable laws. Product offerings and specifications are subject to change without notice. Actual products may vary from photos. Not all products include all features. Availability varies by region; contact your sales representative.

Table of Contents

Table of Contents	3
Introduction	5
Galaxy Integration Overview	5
Product Components	5
Features	5
Installation	7
Minimum Hardware Requirements	7
Installation Prerequisites	7
Installing Galaxy Intrusion Integration to victor	7
Uninstalling the Galaxy Intrusion Integration to victor	7
Configuring Galaxy Panel to Communicate with victor	9
Enabling Engineering Access using the Keypad	9
Entering Engineering Mode using the Keypad	9
Configuring the Galaxy Panel to Receive Events using the Galaxy Keypad	10
Configuring the Galaxy Panel to Always Allow Remote Access	11
Disabling the Encryption	11
Closing Engineering Mode	12
Enabling OMIT State	12
Network Switch Port Settings	12
Firewall Settings	12
Administration	13
General Hardware information	13
victor integration information	13
Adding and Editing Galaxy Intrusion Panels	14
Editing the Galaxy Panels	15
View and Edit Galaxy Partitions	16
View and Edit Galaxy Zones	16
View and Edit Galaxy Outputs	18
View and Edit Galaxy Secondary Devices	19
Configuring Galaxy Alerts	19

Operation	21
Health Dashboard	21
Reports	21
Dynamic Views	21
Manual Actions	21
Panel Synchronization	21
Set and Unset Partitions	22
Activate and Deactivate Outputs	22
Bypass and Reset Zones	23
Accessing Virtual Keypad	23
Acknowledging Alarms Using Virtual Keypad	24
Troubleshooting	25
Appendix A: Alert Types	27
Appendix B: Health Status	35
Appendix C: Galaxy Journal Messages	37
Galaxy Zones Status in victor	41
Appendix D: AllowTamperMessages Config Entry	44

Galaxy Integration Overview


Galaxy Intrusion integration provides advanced, seamless integration between victor unified systems and Honeywell Galaxy Intrusion Security System, allowing users of victor Unified Client to monitor and configure their Galaxy Intrusion device hardware, alarms from the victor environment.

This document describes the Galaxy Intrusion integration from within the victor environment. All the features/functionality explained are with respect to the victor platform.

Product Components

- **Galaxy Client:** Used to specify connection details and synchronization actions to Galaxy panels
- **Galaxy Objects:** Physical or logical Galaxy entities within the victor environment.
- **Galaxy Server Component:** The heart of the integration, facilitates and maintains communication with the Galaxy devices and auto-creates partitions, zones, outputs and secondary devices based on the panel capabilities.
- **Galaxy Intrusion Panel:** Control panel used to detect intrusion in a partition and report the alarm. The Panel types are supported are GD-48, GD-96, GD-264, GD-520.

Figure 1: System Overview: IP Configuration

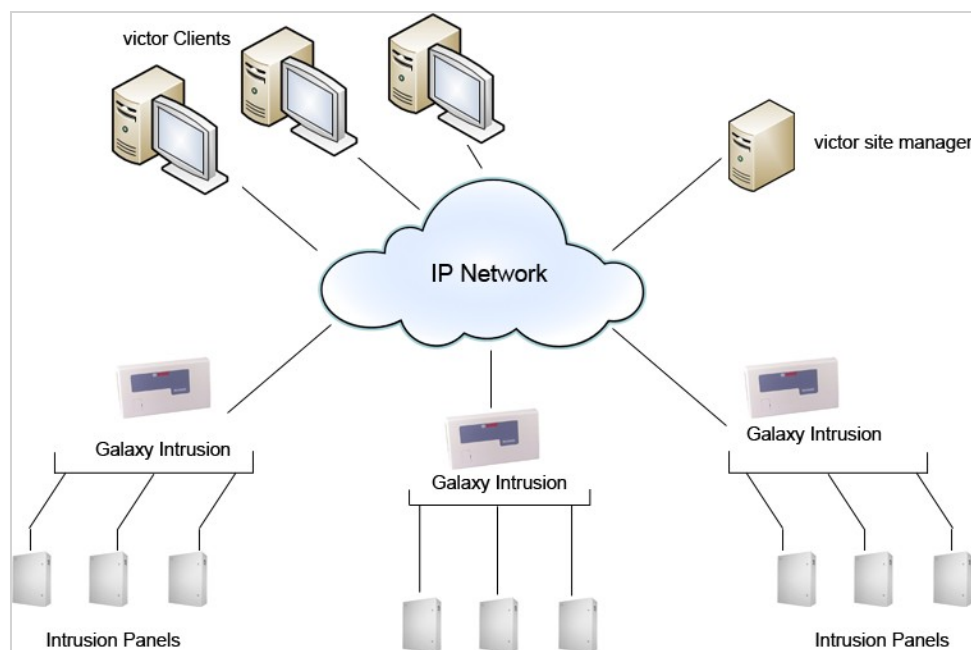

All relevant Galaxy object editors are available from victor's intrusion ribbon bar after driver installation.

Features

The objective of the Galaxy Intrusion integration is to provide a standard, single interface between Galaxy Intrusion devices and American Dynamic's victor Unified Management product.

The following are the features supported:

- Supports GD-48/96/264/520 Panels.
- Supports Manual synchronization of Galaxy objects.

- Supports the following manual actions to control the Galaxy objects.
 - Partition: Set or Unset
 - Zone: Bypass or Reset
 - Output: Activate or Deactivate
- Allows to add new Galaxy Intrusion panels.
- Allows to edit Galaxy Intrusion objects (Panels, Partitions, Zones, Outputs, Secondary devices).
- Allows to view status and information of configured Galaxy devices and objects.
- Supports victor role respect.
- Provides integration with victor Object Association.
- Provides victor Client-side event management.
- Monitor devices on victor Maps and Health dashboard.
- Supports TLS 1.2 for security.

Minimum Hardware Requirements

Galaxy Intrusion integration has the same hardware requirements as victor Unified Client and victor Site Manager. Therefore, if your machine can successfully run victor then it satisfies the requirements for the Galaxy Intrusion Integration.

The integration requires approximately 50MB of hard disk space.

Installation Prerequisites

Prerequisites to install Galaxy Intrusion Integration are:

- To install the Galaxy Intrusion Integration on victor Application Server, you must install the .NET Framework 3.5 on victor server.
- You must install the Galaxy Intrusion driver on both the victor Site Manager and all victor Unified Client machines.
- It is recommended to stop the CrossFire services before initiating the installation of Galaxy Intrusion Integration.

Installing Galaxy Intrusion Integration to victor

- 1 Close all programs.
- 2 Go to <http://www.americandynamics.net>
- 3 Download the appropriate version of the Galaxy Integration Software Driver according to your version of victor.
- 4 Start the Galaxy Integration driver installer. The **End User License Agreement** window appears.
- 5 Select the **I agree to the license terms and conditions** check box, and then click **Install**. For server installations running CrossFire service, the **Tyco CrossFire Service Alert** dialog box appears.
- 6 Click **OK** to continue with the installation. The **Welcome to the Integration Setup Wizard** appears.
- 7 Click **Next** to continue with the installation. The **Installation Options** dialog box appears.
- 8 (Optional) To enable the driver for redundancy, select the **Redundant server installation using supported third party redundancy** check box and enter the Virtual sever (alias) name.
- 9 Click **Next**. The **Ready to Install the Integration** dialog box appears.
- 10 Click **Install**. After a few minutes, the **Completed the Integration Setup Wizard** appears.

Note:

- If you click Cancel, installation is rolled back to clean state.
 - The **Start the Tyco CrossFire services** check box is selected by default. If this check box is not selected, then the CrossFire services will not start automatically
-

- 11 Click **Finish** to complete the installation process. The **Setup Successful** dialog box appears.
- 12 Click **Close** to exit the installation wizard.

Uninstalling the Galaxy Intrusion Integration to victor

- 1 Close all running programs.
- 2 Open **Control Panel** and click **Programs and Features**.
- 3 Right-click **Galaxy** and select **Uninstall**.

- The Modify Setup dialog box appears dialog box opens.
- 4 Click **Uninstall**. The **Drop Database** dialog box appears.
- 5 Select one of the following options:
- Click **Yes** to delete the database used in the Galaxy integration configuration.
 - Click **No** to retain the database used in the Galaxy integration configuration.
- The **Setup Successful** dialog box appears.
- 6 Click **Close** to exit from the uninstallation wizard.

Note:

The Galaxy integration shuts down and restarts the CrossFire services. Therefore, the Galaxy integration uninstall should be planned accordingly.

Configuring Galaxy Panel to Communicate with victor

The following Galaxy Dimension panels are supported:

- Galaxy Ethernet E080-2 firmware version 2.08 and H/W 1.00
- Galaxy Controller panel firmware version v6.10, v6.50, v6.70, v6.79, v6.92 Supported Galaxy Dimension panel models are:

Galaxy Dimension Intrusion Panel	Firmware Version
GD-48	v6.10, v6.50, v6.70, v6.79, v6.92
GD-96	v6.70, v6.79, v6.92
GD-264	v6.70, v6.79, v6.92
GD-520	v6.70, v6.79, v6.92

Enabling Engineering Access using the Keypad

Use the keypad to type the following in the same sequence:

- 1 Open Engineering Menu.
- 2 12345, Ent, Ent, Ent,
- 3 48=ENG. ACCESS, Ent
- 4 1=System Access, Ent
- 5 1=Engineer, Ent
- 6 0=Disabled press 1 to make it 1=Enabled, Ent
- 7 Esc, Esc, Esc

Entering Engineering Mode using the Keypad

Use the keypad to type the following in the same sequence:

- 1 1112233, Ent, Ent
Assign an IP Address and Subnet Mask to the Galaxy Panel
- 2 56=Communication, Ent
- 3 4=Ethernet, Ent
- 4 01=Module Config, Ent
- 5 1=IP Address, Ent
- 6 Type the IP Address to be assigned to the panel. Use # for a dot, B to backspace.
- 7 Press Enter to save the IP Address.
- 8 4=Network Mask, Ent
- 9 Type the Subnet Mask. Use # for a dot, B to backspace.
- 10 Press Enter to save the Subnet mask.
- 11 3=Gateway IP (if required)

- 12 Type the Gateway IP Address. Use # for a dot, B to backspace.
- 13 Press Enter to save the Gateway Address.
- 14 Press Esc.
- 15 Keypad shows 01=Module Config

Configuring the Galaxy Panel to Receive Events using the Galaxy Keypad

Use the keypad to type the following in the same sequence:

- 1 56=Communication, Ent
- 2 4=Ethernet, Ent
- 3 02=Alarm Report, Ent
- 4 1=Format, Ent
- 5 2=Microtech, Ent
- 6 1=Trigger events, Ent.

Note:

There are 20 trigger events and all of them must be ON. To turn on all 20 events, you must set Ent 1=Status Ent 1=ON Ent Esc. Repeat step 5 for all the 20 events.

- 7 Esc, Esc
- 8 2=Primary IP, Ent
- 9 1=IP Address, Ent. Type the IP Address of the computer to which the panel is connected. Use # for a dot, B to backspace.
- 10 Press Enter to save the IP Address.
- 11 2=Port No., Ent.

Note:

The default port number is 10002. Press the B button for backspace. You must change the default port number if you have multiple Galaxy Panels. Each panel should have an unique port number.

- 12 Press Enter to save the Port number.
- 13 4=Account No., Ent. The default setting is 12345. Use to B to backspace.
- 14 Press Enter to save the Account number.
- 15 5=Receiver, Ent
- 16 2=Dual, Ent
- 17 6=Alarm Mon, Ent
- 18 1=Trigger events, Ent

Note:

There are 20 trigger events and all of them must be ON. To turn on all 20 events, you must set Ent 1=Status Ent 1=ON Ent Esc. Repeat step 17 for all the 20 events.

- 19 2=Account No., Ent. Enter the Account number that you configured in step 13. Press Ent.
- 20 Press Enter to save the Account number.
- 21 4=Port Number, Ent. Enter the above configured Port number. Press Ent.
- 22 Press Enter to save the Port number.

Note:

Do not enter an IP address in the Secondary IP field. If you configure a Secondary IP address, then you may experience "Comms Fail Error" on the Galaxy Keypad.

- 23 Esc
- 24 8=Protocol, Ent
- 25 1=TCP, Ent
- 26 Esc, Esc, Esc

Note:

- When there are alarms in the Panel, the status of the Alarm Channel changes to Online. When there are no alarms in the Panel, the status of the Alarm Channel is either Offline or Unknown.
 - Driver will disconnect and reconnect Panel, if valid acknowledgment from the Panel is not received for more than 25 packets.
-

Configuring the Galaxy Panel to Always Allow Remote Access

This is used only in the Galaxy Controller Panel. Use the keypad to type the following in the same sequence:

- 1 Open the Engineering Menu.
- 2 56=Communications, Ent
- 3 4=Ethernet, Ent
- 4 03=Remote Access, Ent
- 5 1=Access Period, Ent
- 6 4=Any Time, Ent
- 7 2=Mode, Ent
- 8 1=Direct Access, Ent
- 9 Esc, Esc, Esc, Esc, Esc

Disabling the Encryption

Use the keypad to type the following in the same sequence:

- 1 Open the Engineering Menu.
- 2 56=Communications, Ent
- 3 4=Ethernet, Ent
- 4 09=Encrypt, Ent
- 5 1=Alarm Report, Ent
- 6 0=it should be set to zero, this indicates OFF, Ent
- 7 2=Remote Access, Ent
- 8 0=it should be set to zero, this indicates OFF, Ent
- 9 3=SIA Control, Ent
- 10 0=it should be set to zero, this indicates OFF, Ent
- 11 4=Alarm Monitoring, Ent
- 12 0=it should be set to zero, this indicates OFF, Ent
- 13 Esc, Esc, Esc, Esc, Esc

14 Exit Engineering Mode

Note:

Close the Engineering Mode before you attempt to receive the events from the panel.

Closing Engineering Mode

Use the keypad to type the following in the same sequence:

- 1 51=PARAMETERS, Ent
- 2 17=Restart, Ent
- 3 1=Restart, Ent, Ent

Enabling OMIT State

Use the keypad to type the following in the same sequence:

- 1 Open Engineering Menu in the Panel
- 2 112233, Ent, Ent, Ent
- 3 52=Program Zone, Ent
- 4 1=Zones, Ent 2=RF Zones, Ent
- 5 Using A/B buttons navigate the zone you wish to omit, Ent
- 6 04=Omit, Ent
- 7 1=Enable, 0=Disable

Network Switch Port Settings

The Galaxy E080 Ethernet port is fixed as a 10Mb Half Duplex interface. Most of the Network equipments detect these settings automatically, but sometimes you must manually configure the port for the Galaxy. Contact your local IT Support group for assistance.

Firewall Settings

To receive alarms, you must add the port in the exception list. For example, if port 10001, which is a command port, is not listed in the exception list of firewall, then the Galaxy Intrusion Panel remains offline in victor.

By default, the command port number is 10001 and Alarm Reporting port number is 10002. Each panel must have a unique port to report alarms and you must add all these ports in the exception list of the firewall.

General Hardware information

Detailed hardware information is available for all configured Galaxy Intrusion devices within victor. To access this information, on the Setup tab in the Intrusion group, click the required object and then select Show All. A new tab opens and all available objects are listed, right-click a desired object and click Edit. This information is also available if you right-click an object on the Device List and click Edit.

victor integration information

Roles

victor roles support Galaxy Intrusion device privileges. All context menu actions that are associated with the devices are added to existing victor roles which can be edited accordingly. For more information on Roles, refer to victor Unified Client / victor Application Server Administration and Configuration Guide.

Associations

victor's Object Association supports Galaxy Intrusion objects. Object Association refers to linking unrelated victor objects with the intent of enabling incident building capability. For more information about Object Associations, refer to the victor Unified Client Configuration and User Guide.

Reports

victor's report selection tool and Find in Journal feature support Galaxy Intrusion objects. For more information on Reports and the Find in Journal feature, refer to the victor Unified Client Configuration and User Guide.

Events

victor Events supports Galaxy Intrusion objects support allowing you to detect, monitor and record specific activities on the system. For further information on Events, refer to the victor Unified Client Configuration and User Guide.

Maps

victor Maps and Find on Map features support Galaxy Intrusion objects. For more information on Maps and the Find on Map feature, refer to the victor Unified Client Configuration and User Guide available on the American Dynamics website www.americandynamics.net

Note:

victor editors offer various save options when creating or editing objects:

- **Save and Close** - Save the current object and close the editor.
 - **Save (Apply)** - Save changes and keep the editor open, so that you can make further changes.
 - **Save and New** - Save the current object and open a new editor to create a new object with default values populated.
 - **Close** - Cancel changes and close the editor without saving.
-

Adding and Editing Galaxy Intrusion Panels

Before you add Partitions, Zones, and Outputs, you should configure new panels using the Galaxy Panel editor.

- 1 Select **Galaxy Panel** from the **Create New Item** screen. The **New Galaxy Panel** opens.
- 2 Click **General**. In the expanded list, add the following details:

Property	Description
Name	Enter a name for the panel in the Name text box.
Description	Enter a description for the panel in the Description text box.
Enabled	By default, the Enabled check box is selected. To deactivate the Panel, clear the check box.

- 3 Click **Panel Configuration**. In the expanded list, add the following details:

Property	Description
Controller Type	This field is read-only. It displays a type of Galaxy Panel. For example: GD, 48,96,116, 520.
Account Number.	Enter the account number. This is used to uniquely identify a Panel. Account number can have 1 - 10 digits and the default value is null.
Panel IP Address	Type the TCP/IP network address of the Galaxy Panel. Note: Ensure that the IP Address is unique and in the IPV4 format, else an error message is displayed.
Remote Command Port	Enter the port number that is used to send and receive data from panel. By default, the command port is 10001. The port number can have 1 - 5 digits.
Host IP Address	Type the TCP/IP network address of the host machine. The address must be in IPv4 format and unique within the system network. Note: When the you upgrade from an older driver version, this field is automatically set to 0.0.0.0 so that the panel comes online irrespective of the NIC. If there are multiple NICs in the host machine, you must configure this field with the Host IP address after upgrading. Ensure that the IP address of the host machine is configured in each Galaxy panel.
Local Alarm Port	Enter the port number that is used to receive alarms from the Panel. The port number can be in the range of 1 to 5 digits. By default, the Local port is 10002. NOTE: The same port number needs to be programmed in respective Galaxy panel. If multiple Galaxy Panels are in use, there should be a unique Alarm port number. If not the error message: The same Alarm Port already exists appears.

- 4 (Optional) Click **Panel Information** to view the following information:

- FirmwareVersionContent
 - Last Synchronization Time
- 5 (Optional) Click **Panel Status** to view the following information:
- Command Channel Status:
 - Online
 - Offline
 - Unknown
 - Alarm Channel Status:
 - Online
 - Offline
 - Unknown
 - Synchronization Status
 - Unknown
 - Synchronizing
 - Synchronized
 - Synchronization failed

Note:

- When there are alarms in the Panel, the status of the AlarmChannel changes to Online. When there are no alarms in the Panel, the status of the AlarmChannel is either Offline or Unknown.
 - Driver will disconnect and reconnect panel, if valid ack from the panel is not received for more than 25 packets.
-

- 6 Click **Associations**:
- a Click  to open the Object Selector.
 - b From the **Type** list in the Object Selector, select an object to associate it with the Galaxy panel.
 - c Click **OK**.
- 7 Click **Save**.

Editing the Galaxy Panels

You can configure server connection details from within victor, using the Galaxy Panel editor. For more information, see "Adding and Editing Galaxy Intrusion Panels".

- 1 Select **Galaxy Panel** from **Edit Existing Item** screen.
- 2 Click the **Galaxy Panel** to be edited.
- 3 Click **General**. In the expanded list, edit the required details.
- 4 Click **Panel Configuration**. In the expanded list, edit the required details.
- 5 Click **Panel Information** to view more details.
- 6 Click **Panel Status** to view more details.
- 7 Click **Associations**. Use the Object Selector to associate other hardware devices with the Galaxy panel.
- 8 Click **Save**.

View and Edit Galaxy Partitions

Depending on your victor Role assignment, you can view and edit Galaxy Partitions but cannot create Partitions directly from victor.

- 1 Select **Galaxy Partition** from **Show all Items** screen.
- 2 The **Galaxy Partitions** tab opens and a list containing all available Partitions is displayed.
- 3 To Edit Partitions, select **Galaxy Partition** from **Edit Existing Item** screen.
- 4 Click **General**. In the expanded list, edit the required details:

Property	Description
Name	Enter or edit the name for the Partition.
Description	Enter or edit the description for the Partition.
Enabled	By default, the Enabled check box is selected.

- 5 Click **Partition Information** to view the **Group Number**.
- 6 Click **Partition Zone Mapping** to view the following details:

Property	Description
Zone Name	This field is read-only. Auto generated based on synchronized zones
Zone Number	This field is read-only. Auto generated based on synchronized zones.
Zone Type	This field is read-only. Auto generated based on synchronized zones.
Board	This field is read-only. Auto generated based on synchronized zones.

- 7 Click **Partition Status** to view the Mode Status.
- 8 Click **Save**.

View and Edit Galaxy Zones

Depending on your victor Role assignment, you can view and edit Zones but cannot create Zones directly from victor.

- 1 Select **Galaxy Zone** from **Show all Items** screen.
- 2 The **Galaxy Zones** tab opens and a list containing all available zones is displayed.
- 3 To Edit Zones, select **Galaxy Zone** from **Edit Existing Item** screen.
- 4 Click **General**. In the expanded list, edit the required details:

Property	Description
Name	Enter or edit the name for the Zone.
Description	Enter or edit the description for the Zone.
Enabled	By default, the Enabled check box is selected.

- 5 Click **Zone Information**. In the expanded list, edit the required details:

Property	Value
Zone number	This field is read-only. Auto generated based on synchronized zones.
Zone Type	This field is read-only. Displays the synchronized value for each zone.
Board	This field is read-only. Displays the synchronized value for each zone.
Send state changes to Activity Viewer	Select this check box to send state changes to Activity Viewer.
Send state changes to Journal	Select this check box to send state changes to Journal.

- 6 Click **Zone Status** to view the following:

Property	Value
Active Status	The possible values are: • Active • Inactive
Hardware Status	The possible values are: • Closed • Open • Short Circuit • Low Resistance • Masked • Faulted

Property	Value
Alarm Status	The possible values are: • Normal • Alarm
Supervision Status	The possible values are: • Close • Loop • Open Loop • Tamper • Trouble • Zone Masked • Zone Faulted • Bypass • Suspended • Soak Test • Reset

- 7 Click **Save**.

View and Edit Galaxy Outputs

Depending on your victor Role assignment, you can view and edit Outputs but you cannot create Outputs directly from victor.

- 1 Select **Galaxy Output** from **Show all Items** screen. The Galaxy Outputs tab opens and a list containing all available Outputs are displayed.
- 2 To Edit Outputs, select **Galaxy Zone** from **Edit Existing Item** screen. A new tab opens.
- 3 Click **General**. In the expanded list, edit the required details:

Property	Description
Name	Enter or edit the name for the Output
Description	Enter or edit the description for the Output.
Enabled	By default, the Enabled check box is selected.

- 4 Click **Output Information**. In the expanded list, edit the required details:

Property	Value
Output number	This field is read-only.

Property	Value
	Auto generated based on synchronized outputs.
Output Type	This field is read-only. Displays the synchronized value for each zone.
Board	This field is read-only. Displays the synchronized value for each zone.
Send state changes to Activity Viewer	Select this check box to send state changes to Activity Viewer.
Send state changes to Journal	Select this check box to send state changes to Journal.

5 Click **Output Status** to view whether the Active Status.

6 Click **Save**.

View and Edit Galaxy Secondary Devices

Depending on your victor Role assignment, you can view and edit Secondary Devices but cannot create Secondary Devices directly from victor.

- 1 Select **Galaxy Secondary Device** from **Show all Items** screen. The **Galaxy Secondary Devices** tab opens and a list containing all available secondary devices are displayed.
- 2 To Edit Secondary Devices, select **Galaxy Secondary Device** from **Edit Existing Item** screen.
- 3 Click **General**. In the expanded list, edit the required details:

Property	Description
Name	Enter or edit the name for the secondary device.
Description	Enter or edit the description for the secondary device.
Enabled	By default, the Enabled check box is selected.

4 Click the **Secondary Device Information** to view the Device Number.


5 Click the **Secondary Device Zones** to view the zone information that is mapped to the secondary devices.

6 Click the **Secondary Device Output** to view the output information that is mapped to the secondary devices.

7 Click **Save**.

Configuring Galaxy Alerts


You can use the Event Setup editor to configure alerts for Galaxy Panels, Alerts, Zones and Outputs. You can configure alerts for Communication Status, Synchronization Status, and Trouble Status properties of panels.

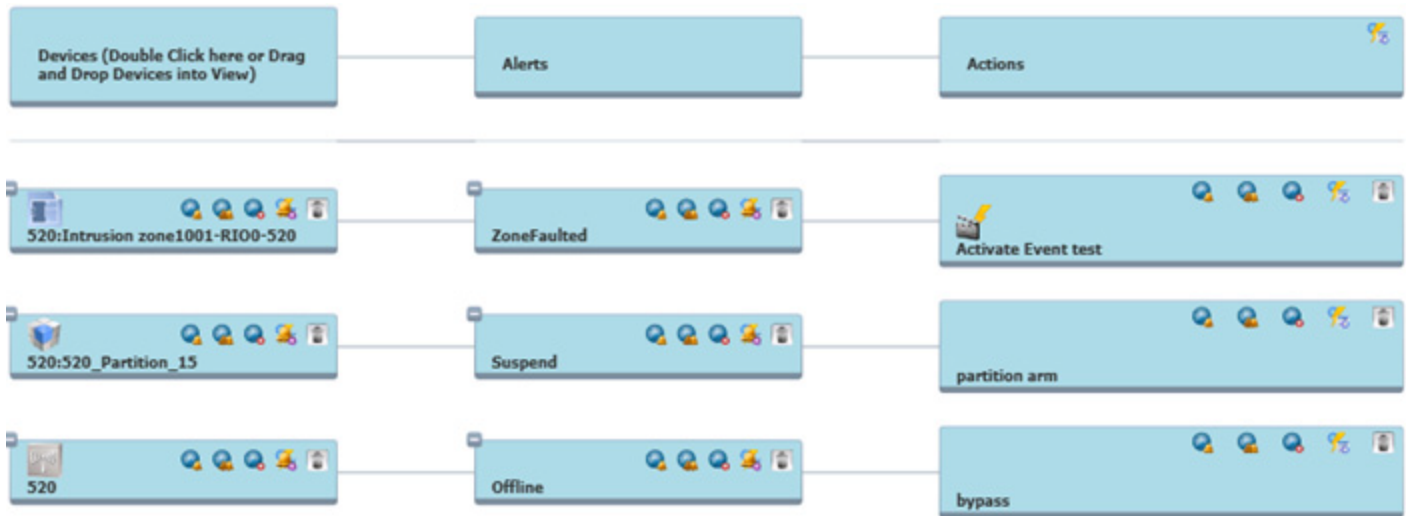

Refer to [Alert Types on page 29](#) for a full list of victor support alert types.

Health Dashboard

The health status of all Galaxy objects is annunciated in victor's Health Dashboard as follows:

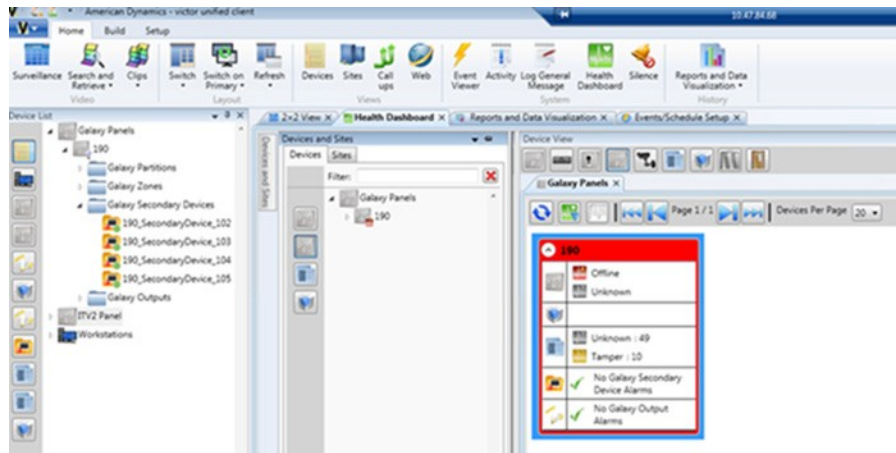

Refer to Health Status on page 29 for a full list of supported health statuses.

Reports

You can use the victor journal type Journal Intrusion Message to search for Galaxy related report entries as detailed below:

For more information on reporting within victor, refer to the victor Unified Client / victor Application Server Administration and Configuration Guide.

Dynamic Views


All configured Galaxy Panels, Zones, Partition and Outputs can be displayed in victor's object list views (dynamic views). From here you can perform manual actions on configured objects.

Manual Actions

You can perform various manual actions from within victor client:

Panel Synchronization

You can synchronize Galaxy panels directly from the victor device list.

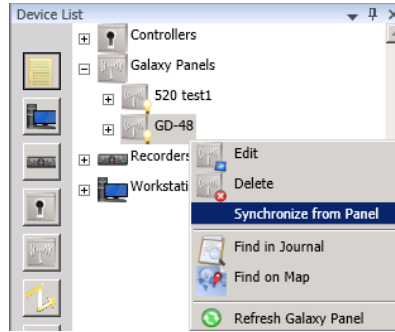


- Select **Right Click>Synchronize** (Panel UI is disabled during synchronization)

Set and Unset Partitions

You can set or unset partitions directly from the victor device list.


- To set the partition, right-click the partition and select **Set**.
- To unset the armed partition, right-click the partition and select **Unset**.

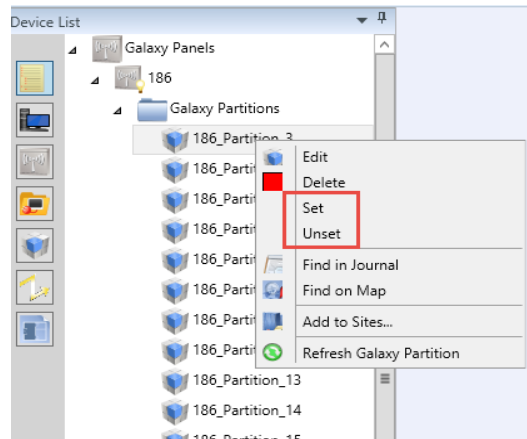

Activate and Deactivate Outputs

You can activate and deactivate outputs directly from the victor device list.


- To activate the output, right-click the output and select **Activate**.
- To deactivate the output, right-click the output and select **Deactivate**.

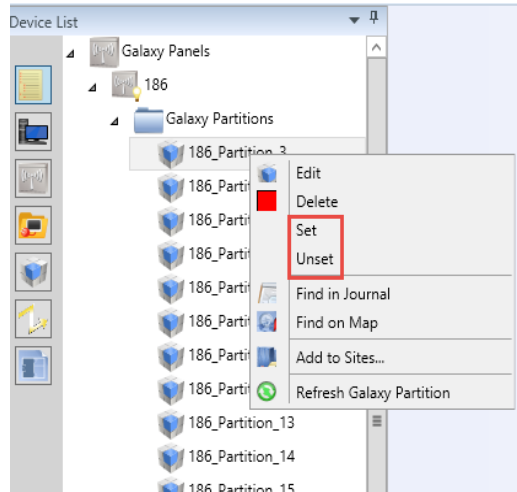

Bypass and Reset Zones

You can bypass and reset zones directly from the victor device list.

- To bypass the zone, right-click the zone and select **Bypass**.
- To reset the zone, right-click the zone and select **Reset**.

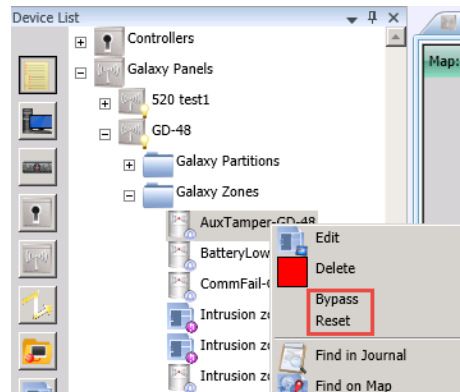


Accessing Virtual Keypad

Virtual keypad is used to acknowledge alarms. Follow the steps to access the virtual keypad:

- In the **Device List**, expand the **Galaxy Panels** folder.
- Right-click a panel and click **Virtual Keypad**.

Figure 2: Accessing Virtual Keypad

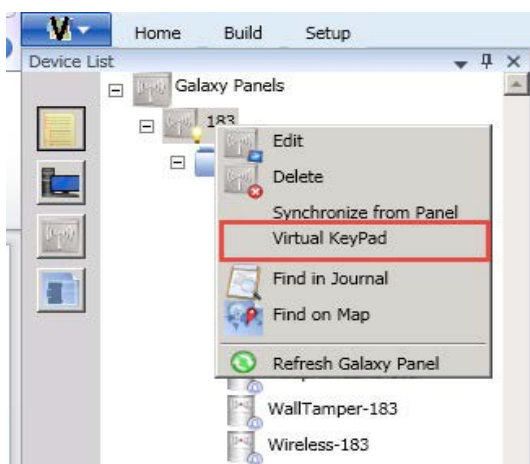


Note:

On the context menu, the virtual keypad option is available only if:

- The Panel is online or enabled
- Synchronization is not in progress

The virtual keypad opens as shown in the following image:

Figure 3: Virtual Keypad

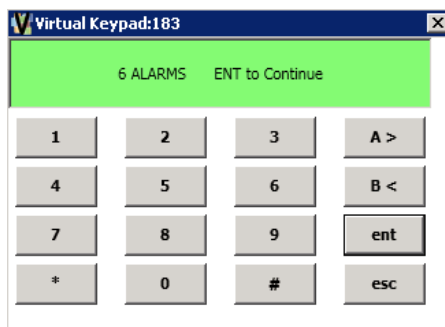

Note:

You can access either the physical keypad or the virtual keypad but cannot access both the keypads simultaneously.

- On a victor client, you can launch only one virtual keypad at a time.
- On a server or remote clients, you can launch multiple virtual keypads. If multiple virtual keypads are launched, the activity performed on one virtual keypad is reflected on all virtual keypads. Hence this is not recommended.
- Virtual Keypad closes automatically in the following scenarios:
 - When you perform manual action on Galaxy objects.
 - If the Panel goes offline.
 - If the Panel is disabled.

Acknowledging Alarms Using Virtual Keypad

Follow the steps to acknowledge alarms using virtual keypad:

- 1 Enter the Valid User code with the sufficient level to reset the alarm.
- 2 Press **Ent** to clear the alarms.

This section provides troubleshooting information for issues that may occur in the victor Galaxy Integration.


Problem:

Sometimes the installation may fail if the CrossFire service does not stop on time and throws a time out error.

Solution:

Ensure that you have completed the following steps:

- Check if the CrossFire service is stopped from services panel in case of installation failure. Refer to the following image:

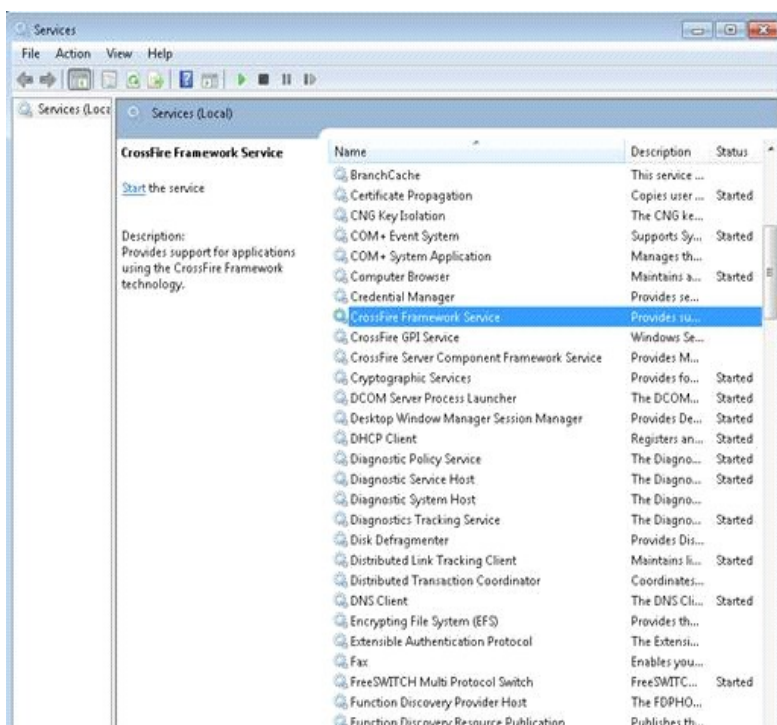

- Wait till the CrossFire service is stopped and then trigger the installation again. This will work fine as the service is stopped already.

Problem:

Occasionally Partition does not get Set

Solution:

This occurs if one or more zones in the partition are not in a normal condition. Check for the zone status in that partition and restore the state of the zone to normal.

OR

This occurs when multiple Partitions are selected and the user performs a Set/Unset manual action. In order to Set/Unset the Partition, it is recommended that you add the Partitions to a group and then perform a Set/Unset manual action on that group.

Problem:

The Galaxy Panel does not connect.

Solution:

Ensure that you have completed the following:

- Configure the Panel as per the instructions in Configuring Galaxy Panel to Communicate with victor.
- Check your firewall settings and ensure ports configured in the panel are opened.
- Disable the panel in victor and telnet to the panel on Command Port.

Problem:

Alarms are not received from the Panel.

Solution:

Complete the following:

- Check your firewall settings and ensure ports configured in the panel are opened.
- Configure the Panel as per the instructions in Configuring Galaxy Panel to Communicate with victor.

Appendix A: Alert Types

Use the Event Configuration editor to configure alerts for Galaxy objects. The following tables list the Galaxy object Alert Types that are supported in victor:

Table 1: Alert Types for Galaxy Panels

Panel Alert Type	Value
Online Status	Online
	Offline
	Disabled
Synchronization Status	Synchronizing
	Synchronized
	Synchronization Failed

Table 2: Alert Types for Galaxy Partitions

Partition Alert Type	Value
Armed State	Unknown
	Armed
	Disarmed
	Unset
	Setting
	Suspend
	Set
	Unsetting
	PartSetAndUnset
	AlarmAndUnset
	SystemAndUnset
	PAAAlarmAndUnset
	TamperAndUnset
	PartSetAndSetting
	AlarmAndSetting
	SystemAndSetting

Partition Alert Type	Value
	PAArmAndSetting TamperAndSetting PartSetAndSuspend AlarmAndSuspend SystemAndSuspend PAArmAndSuspend TamperAndSuspend PartSetAndSet AlarmAndSet SystemAndSet PAArmAndSet TamperAndSet PartSetAndUnsetting AlarmAndUnsetting SystemAndUnsetting PAArmAndUnsetting TamperAndUnsetting
Armed State	PartSetAlarmAndUnset PartSetSystemAndUnset PartSetPAArmAndUnset PartSetTamperAndUnset PartSetAlarmAndSetting PartSetSystemAndSetting PartSetPAArmAndSetting PartSetTamperAndSetting PartSetAlarmAndSuspend PartSetSystemAndSuspend PartSetPAArmAndSuspend PartSetTamperAndSuspend PartSetAlarmAndSet

Partition Alert Type	Value
	PartSetSystemAndSet PartSetPAAAlarmAndSet PartSetTamperAndSet, PartSetAlarmAndUnsetting PartSetSystemAndUnsetting PartSetPAAAlarmAndUnsetting PartSetTamperAndUnsetting AlarmSystemAndUnset AlarmPAAAlarmAndUnset AlarmTamperAndUnset AlarmSystemAndSetting AlarmPAAAlarmAndSetting AlarmTamperAndSetting AlarmSystemAndSuspend AlarmPAAAlarmAndSuspend AlarmTamperAndSuspend AlarmSystemAndSet AlarmPAAAlarmAndSet AlarmTamperAndSet AlarmSystemAndUnsetting
Armed State	AlarmPAAAlarmAndUnsetting AlarmTamperAndUnsetting SystemPAAAlarmAndUnset SystemTamperAndUnset SystemPAAAlarmAndSetting SystemTamperAndsetting SystemPAAAlarmAndSuspend SystemTamperAndSuspend SystemPAAAlarmAndSet SystemTamperAndSet

Partition Alert Type	Value
	SystemPAAAlarmAndUnsetting SystemTamperAndUnsetting PartSetAlarmSystemAndUnset PartSetAlarmPAAAlarmAndUnset PartSetAlarmTamperAndUnset PartSetAlarmSystemAndSetting PartSetAlarmPAAAlarmAndSetting PartSetAlarmTamperAndSetting PartSetAlarmSystemAndSuspend PartSetAlarmPAAAlarmAndSuspend PartSetAlarmTamperAndSuspend PartSetAlarmSystemAndSet PartSetAlarmPAAAlarmAndSet PartSetAlarmTamperAndSet PartSetAlarmSystemAndUnsetting PartSetAlarmPAAAlarmAndUnsetting PartSetAlarmTamperAndUnsetting, PartSetAlarmSystemTamperAndUnset PartSetAlarmSystemTamperAndsetting PartSetAlarmSystemTamperAndSuspend
Armed State	PartSetAlarmSystemTamperAndSet PartSetAlarmSystemTamperAndUnsetting PartSetAndAlarm PartSetAndSystem PartSetAndPAAAlarm PartSetAndTamper AlarmAndSystem AlarmAndPAAAlarm AlarmAndTamper SystemAndPAAAlarm

Partition Alert Type	Value
	SystemAndTamper PartSetAlarmSystemPAAalarmAndTamper PartSetAlarmSystemPAAalarmAndUnset PartSetAlarmSystemPAAalarmAndSetting PartSetAlarmSystemPAAalarmAndSuspend PartSetAlarmSystemPAAalarmAndSet PartSetAlarmSystemPAAalarmAndUnsetting AlarmSystemPAAalarmTamperAndUnset AlarmSystemPAAalarmTamperAndSetting AlarmSystemPAAalarmTamperAndSuspend AlarmSystemPAAalarmTamperAndSet AlarmSystemPAAalarmTamperAndUnsetting AlarmSystemPAAalarmAndUnset AlarmSystemAndPAAalarmAndSetting AlarmSystemAndPAAalarmAndSuspend AlarmSystemAndPAAalarmAndSet, AlarmSystemAndPAAalarmAndUnsetting PartSetSystemPAAalarmAndUnset PartSetSystemPAAalarmAndSetting PartSetSystemPAAalarmAndSuspend
Armed State	PartSetSystemPAAalarmAndSet PartSetSystemPAAalarmAndUnsetting PAAalarmTamperAndUnset PAAalarmTamperAndSetting PAAalarmTamperAndSuspend PAAalarmTamperAndSet PAAalarmTamperAndUnsetting SystemPAAalarmTamperAndUnset SystemPAAalarmTamperAndSetting SystemPAAalarmTamperAndSuspend

Partition Alert Type	Value
	SystemPAAAlarmTamperAndSet SystemPAAAlarmTamperAndUnsetting AlarmPAAAlarmTamperAndUnset AlarmPAAAlarmTamperAndSetting AlarmPAAAlarmTamperAndSuspend AlarmPAAAlarmTamperAndSet AlarmPAAAlarmTamperAndUnsetting AlarmSystemTamperAndUnset AlarmSystemTamperAndsetting AlarmSystemTamperAndSuspend AlarmSystemTamperAndSet AlarmSystemTamperAndUnsetting PartSetPAAAlarmTamperAndUnset PartSetPAAAlarmTamperAndSetting PartSetPAAAlarmTamperAndSuspend PartSetPAAAlarmTamperAndSet PartSetPAAAlarmTamperAndUnsetting PartSetSystemTamperAndUnset PartSetSystemTamperAndsetting PartSetSystemTamperAndSuspend
Armed State	PartSetSystemTamperAndSet PartSetSystemTamperAndUnsetting PartSetPAAAlarmSystemTamperAndUnset PartSetPAAAlarmSystemTamperAndsetting PartSetPAAAlarmSystemTamperAndSuspend PartSetPAAAlarmSystemTamperAndSet PartSetPAAAlarmSystemTamperAndUnsetting PartSetAlarmPAAAlarmTamperAndUnset PartSetAlarmPAAAlarmTamperAndSetting PartSetAlarmPAAAlarmTamperAndSuspend

Partition Alert Type	Value
	PartSetAlarmPAAAlarmTamperAndSet PartSetAlarmPAAAlarmTamperAndUnsetting

Table 3: Alert Types for Galaxy Zones

Zone Alert Type	Value
AlarmStatus	Alarm Alarm Restore
Active Status	Active Inactive Disabled
Hardware Status	Closed Open Short Circuit Open Circuit Low Resistance High Resistance Masked Faulted
Supervision Status	Zone Masked Zone Faulted Zone Supervision Fail Bypass Suspended Soak Test Reset Closed Loop Open Loop Trouble Tamper

Zone Alert Type	Value
	Soak Test and Omitted

Appendix B: Health Status

The following tables list the Galaxy object Health status announcements that are supported in victor.

Table 4: Health status for Galaxy Panels

Panel Status	Health Status
Online Synchronized Synchronizing	Normal
Offline SynchronizationFailed	Device Alert
Disabled Unknown	Unknown

Table 5: Health status for Galaxy Partitions

Partition Status	Health Status
Setting/ Unset/ Unsetting/ Set/ Suspend/ Armed/ Disarmed	Normal
AlarmAndSet / AlarmSystemAndSet / TamperAndSet / AlarmTamperAndSet / SystemTamperAndSet / PartSetAndTamper / AlarmAndTamper / SystemAndTamper / PAAAlarmTamperAndSet / AlarmPAAAlarmTamperAndSet / AlarmSystemTamperAndSet / SystemPAAAlarmTamperAndSet / AlarmTamperAndUnset / SystemTamperAndUnset / AlarmSystemTamperAndSuspend / AlarmAndPAAAlarm / AlarmAndSuspend / AlarmAndSystem / AlarmAndUnset / AlarmPAAAlarmAndSet / AlarmPAAAlarmAndUnset / AlarmPAAAlarmTamperAndUnset / AlarmSystemAndPAAAlarmAndSuspend / AlarmSystemAndSetting / AlarmSystemAndUnset / AlarmSystemPAAAlarmAndUnset / AlarmSystemPAAAlarmTamperAndSetting / AlarmSystemPAAAlarmTamperAndSet / AlarmSystemPAAAlarm TamperAndUnset / AlarmSystemTamperAndsetting / AlarmSystemTamperAndUnset / AlarmTamperAndSuspend / PAAAlarmAndUnset / PAAAlarmTamperAndSuspend / PAAAlarmTamperAndUnset / PartSetAndPAAAlarm / PartSetAlarmAndSet / PartSetAlarmAndUnset / PartSetAlarmPAAAlarmAndSet / PartSetAlarmPAAAlarmTamperAndUnset / PartSetAlarmSystemPAAAlarmAndSet / PartSetAlarmSystemPAAAlarmAndTamper / PartSetAlarmSystemTamperAndSet / PartSetAlarmSystemTamperAndUnset / PartSetAlarmTamperAndSet / PartSetAlarmTamperAndUnset / PartSetPAAAlarmAndSet / PartSetTamperAndSet / PartSetTamperAndUnset / PartSetSystemTamperAndUnset / PartSetSystemTamperAndSet / PartSetSystemPAAAlarmAndUnset / PartSetSystemPAAAlarmAndSet	At Risk
Unknown	Unknown

Table 6: Health status for Galaxy Zones

Zone Status	Value
ClosedLoop / Closed / Active / NORMAL	Normal
Tamper / Trouble / ShortCircuit / Open / OpenCircuit / LowResistance / HighResistance / Masked / Faulted	At Risk
Inactive / Disabled / Alarm	Device Alert
Unknown	Unknown

Table 7: Health status for Galaxy Outputs

Output Status	Value
Inactive / Active	Normal

Table 8: Health status for Galaxy Outputs

Output Status	Value
Normal/ModuleRestored	Normal
Tamper/Trouble	AT_RISK
ModuleMissing	Device Alert
Unknown	Unknown

Appendix C: Galaxy Journal Messages

The following table lists the Journal messages that are reported by the Galaxy Integration products to the victor database:

Table 9: Journal Messages Reported to victor by the Galaxy Integration

Hardware Status	Alarm Status	Supervision Status	Condition	Activity Viewer/Journal Message
CLOSED	Normal	Closed Loop	Acknowledged and not omitted	Changes in any/combination of the status (Hardware/Alarm/Supervision status) will reflect in Activity Viewer/Journal
OPEN	Normal	Open Loop	Acknowledged	Changes in any/combination of the status (Hardware/Alarm/Supervision status) will reflect in Activity Viewer/Journal
SHORT CIRCUIT	Normal	Tamper	Acknowledged	Changes in any/combination of the status (Hardware/Alarm/Supervision status) will reflect in Activity Viewer/Journal
OPEN CIRCUIT	Normal	Tamper	Acknowledged	Changes in any/combination of the status (Hardware/Alarm/Supervision status) will reflect in Activity Viewer/Journal
LOW RESISTANCE	Normal	Tamper	Acknowledged	Changes in any/combination of the status (Hardware/Alarm/Supervision status) will reflect in Activity Viewer/Journal
HIGH RESISTANCE	Normal	Trouble	Acknowledged	Changes in any/combination of the status (Hardware/Alarm/Supervision status) will reflect in Activity Viewer/Journal
MASKED	Normal	Zone Masked	Acknowledged	Changes in any/combination of the status (Hardware/Alarm/Supervision status) will reflect in Activity Viewer/Journal
FAULT	Normal	Zone Faulted	Acknowledged	Changes in any/combination of the status (Hardware/Alarm/Supervision status) will reflect in Activity Viewer/Journal
CLOSED	Alarm	Closed Loop	Alarm	Changes in any/combination of the status (Hardware/Alarm/Supervision status) will reflect in Activity Viewer/Journal
OPEN	Alarm	Open Loop	Alarm	Changes in any/combination of the status (Hardware/Alarm/Supervision status) will reflect in Activity Viewer/Journal

Hardware Status	Alarm Status	Supervision Status	Condition	Activity Viewer/Journal Message
SHORT CIRCUIT	Alarm	Tamper	Alarm	Changes in any/combination of the status (Hardware/Alarm/Supervision status) will reflect in Activity Viewer/Journal
OPEN CIRCUIT	Alarm	Tamper	Alarm	Changes in any/combination of the status (Hardware/Alarm/Supervision status) will reflect in Activity Viewer/Journal
HIGH RESISTANCE	Alarm	Trouble	Alarm	Changes in any/combination of the status (Hardware/Alarm/Supervision status) will reflect in Activity Viewer/Journal
MASKED	Alarm	Zone Masked	Alarm	Changes in any/combination of the status (Hardware/Alarm/Supervision status) will reflect in Activity Viewer/Journal
FAULT	Alarm	Zone Faulted	Alarm	Changes in any/combination of the status (Hardware/Alarm/Supervision status) will reflect in Activity Viewer/Journal
CLOSED	Normal	Bypass	Acknowledged and omitted	Changes in any/combination of the status (Hardware/Alarm/Supervision status) will reflect in Activity Viewer/Journal
OPEN	Normal	Bypass	Acknowledged	Changes in any/combination of the status (Hardware/Alarm/Supervision status) will reflect in Activity Viewer/Journal
SHORT CIRCUIT	Normal	Bypass	Acknowledged	Changes in any/combination of the status (Hardware/Alarm/Supervision status) will reflect in Activity Viewer/Journal
OPEN CIRCUIT	Normal	Bypass	Acknowledged	Changes in any/combination of the status (Hardware/Alarm/Supervision status) will reflect in Activity Viewer/Journal
LOW RESISTANCE	Normal	Bypass	Acknowledged	Changes in any/combination of the status (Hardware/Alarm/Supervision status) will reflect in Activity Viewer/Journal
HIGH RESISTANCE	Normal	Bypass	Acknowledged	Changes in any/combination of the status (Hardware/Alarm/Supervision status) will reflect in Activity Viewer/Journal
MASKED	Normal	Bypass	Acknowledged	Changes in any/combination of the status (Hardware/Alarm/Supervision status) will reflect in Activity Viewer/Journal

Hardware Status	Alarm Status	Supervision Status	Condition	Activity Viewer/Journal Message
FAULT	Normal	Bypass	Acknowledged	Changes in any/combination of the status (Hardware/Alarm/Supervision status) will reflect in Activity Viewer/Journal
CLOSED	Normal	Suspended		Changes in any/combination of the status (Hardware/Alarm/Supervision status) will reflect in Activity Viewer/Journal
OPEN	Normal	Suspended		Changes in any/combination of the status (Hardware/Alarm/Supervision status) will reflect in Activity Viewer/Journal
SHORT CIRCUIT	Normal	Suspended		Changes in any/combination of the status (Hardware/Alarm/Supervision status) will reflect in Activity Viewer/Journal
OPEN CIRCUIT	Normal	Suspended		Changes in any/combination of the status (Hardware/Alarm/Supervision status) will reflect in Activity Viewer/Journal
LOW RESISTANCE	Normal	Suspended		Changes in any/combination of the status (Hardware/Alarm/Supervision status) will reflect in Activity Viewer/Journal
HIGH RESISTANCE	Normal	Suspended		Changes in any/combination of the status (Hardware/Alarm/Supervision status) will reflect in Activity Viewer/Journal
MASKED	Normal	Suspended		Changes in any/combination of the status (Hardware/Alarm/Supervision status) will reflect in Activity Viewer/Journal
FAULT	Normal	Suspended		Changes in any/combination of the status (Hardware/Alarm/Supervision status) will reflect in Activity Viewer/Journal
CLOSED	Normal	SoakTest		Changes in any/combination of the status (Hardware/Alarm/Supervision status) will reflect in Activity Viewer/Journal
OPEN	Normal	SoakTest		Changes in any/combination of the status (Hardware/Alarm/Supervision status) will reflect in Activity Viewer/Journal
SHORT CIRCUIT	Normal	SoakTest		Changes in any/combination of the status (Hardware/Alarm/Supervision status) will reflect in Activity Viewer/Journal

Hardware Status	Alarm Status	Supervision Status	Condition	Activity Viewer/Journal Message
OPEN CIRCUIT	Normal	SoakTest		Changes in any/combination of the status (Hardware/Alarm/Supervision status) will reflect in Activity Viewer/Journal
LOW RESISTANCE	Normal	SoakTest		Changes in any/combination of the status (Hardware/Alarm/Supervision status) will reflect in Activity Viewer/Journal
HIGH RESISTANCE	Normal	SoakTest		Changes in any/combination of the status (Hardware/Alarm/Supervision status) will reflect in Activity Viewer/Journal
MASKED	Normal	SoakTest		Changes in any/combination of the status (Hardware/Alarm/Supervision status) will reflect in Activity Viewer/Journal
FAULT	Normal	SoakTest		Changes in any/combination of the status (Hardware/Alarm/Supervision status) will reflect in Activity Viewer/Journal
CLOSED	Normal	Reset	Reset manual action from victor	Changes in any/combination of the status (Hardware/Alarm/Supervision status) will reflect in Activity Viewer/Journal
OPEN	Normal	Reset	Reset manual action from victor	Changes in any/combination of the status (Hardware/Alarm/Supervision status) will reflect in Activity Viewer/Journal
SHORT CIRCUIT	Normal	Reset	Reset manual action from victor	Changes in any/combination of the status (Hardware/Alarm/Supervision status) will reflect in Activity Viewer/Journal
OPEN CIRCUIT	Normal	Reset	Reset manual action from victor	Changes in any/combination of the status (Hardware/Alarm/Supervision status) will reflect in Activity Viewer/Journal
LOW RESISTANCE	Normal	Reset	Reset manual action from victor	Changes in any/combination of the status (Hardware/Alarm/Supervision status) will reflect in Activity Viewer/Journal
HIGH RESISTANCE	Normal	Reset	Reset manual action from victor	Changes in any/combination of the status (Hardware/Alarm/Supervision status) will reflect in Activity Viewer/Journal
MASKED	Normal	Reset	Reset manual action from victor	Changes in any/combination of the status (Hardware/Alarm/Supervision status) will reflect in Activity Viewer/Journal

Hardware Status	Alarm Status	Supervision Status	Condition	Activity Viewer/Journal Message
FAULT	Normal	Reset	Reset manual action from victor	Changes in any/combination of the status (Hardware/Alarm/Supervision status) will reflect in Activity Viewer/Journal

When an area is disarmed and the zone under that area is bypassed, Supervision status of that zone is reset.

Galaxy Zones Status in victor

The priority of icons displayed for Galaxy Zones in victor is as follows:

- 1 Disabled
- 2 Alarm
- 3 Bypass
- 4 Active/Inactive
- 5 Supervision Status
- 6 Open/Closed
- 7 Unknown

The following table lists details about the input statuses in victor and the Status Images assigned to them. Active or Inactive status is displayed only for the conditions displayed in this table.

Table 10: Input Status in victor

Status	Input Status in victor				
	Active Status	Hardware Status	Alarm Status	Supervision Status	Status Image
Alarmed and Open	Active	Open	Alarm	Open Loop	Active
Alarmed and Short Circuited	Active	Short Circuit	Alarm	Tamper	Active
Alarmed and Open Circuited	Active	Open Circuit	Alarm	Tamper	Active
Alarmed and Low Resistance	Active	Low Resistance	Alarm	Trouble	Active
Alarmed and High Resistance	Active	High Resistance	Alarm	Trouble	Active
Alarmed and Masked	Active	Masked	Alarm	Zone Masked	Active
Alarmed and Faulted	Active	Fault	Alarm	Zone Faulted	Active
Omitted	Inactive	Closed	Normal	Bypass	Bypass

Status	Input Status in victor				
	Active Status	Hardware Status	Alarm Status	Supervision Status	Status Image
Omitted and Open	Inactive	Open	Normal	Bypass	Bypass
Omitted and Short Circuited	Inactive	Short Circuit	Normal	Bypass	Bypass
Omitted and Open Circuited	Inactive	Open Circuit	Normal	Bypass	Bypass
Omitted and Low Resistance	Inactive	Low Resistance	Normal	Bypass	Byass
Omitted and High Resistance	Inactive	High Resistance	Normal	Bypass	Bypass
Omitted and Masked	Inactive	Masked	Normal	Bypass	Bypass
Omitted and Faulted	Inactive	Fault	Normal	Bypass	Bypass
Suspended	Inactive	Closed	Normal	Suspended	Inactive
Suspended and Open	Inactive	Open	Normal	Suspended	Inactive
Suspended and Short Circuited	Inactive	Short Circuit	Normal	Suspended	Inactive
Suspended and Open Circuited	Inactive	Open Circuit	Normal	Suspended	Inactive
Suspended and Low Resistance	Inactive	Low Resistance	Normal	Suspended	Inactive
Suspended and High Resistance	Inactive	High Resistance	Normal	Suspended	Inactive
Suspended and Masked	Inactive	Masked	Normal	Suspended	Inactive
Suspended and Faulted	Inactive	Fault	Normal	Suspended	Inactive
Soak Test	Inactive	Closed	Normal	Soak Test	Inactive
Soak Test and Short Circuited	Inactive	Short Circuit	Normal	Soak Test	Inactive
Soak Test and Open Circuited	Inactive	Open Circuit	Normal	Soak Test	Inactive
Soak Test and Low Resistance	Inactive	Low Resistance	Normal	Soak Test	Inactive
Soak Test and High Resistance	Inactive	High Resistance	Normal	Soak Test	Inactive

Status	Input Status in victor				
	Active Status	Hardware Status	Alarm Status	Supervision Status	Status Image
Soak Test and Masked	Inactive	Masked	Normal	Soak Test	Inactive
Soak Test and Faulted	Inactive	Fault	Normal	Soak Test	Inactive
Soak Test, Omitted, and Closed	Inactive	Closed	Normal	Bypass	Inactive
Soak Test, Omitted, and Open	Inactive	Open	Normal	Bypass	Inactive
Soak Test, Omitted, and Short Circuited	Inactive	Short Circuit	Normal	Bypass	Inactive
Soak Test, Omitted, and Open Circuited	Inactive	Open Circuit	Normal	Bypass	Inactive
Soak Test, Omitted, and Low Resistance	Inactive	Low Resistance	Normal	Bypass	Inactive
Soak Test, Omitted, and High Resistance	Inactive	High Resistance	Normal	Bypass	Inactive
Soak Test, Omitted, and Masked	Inactive	Masked	Normal	Bypass	Inactive
Soak Test, Omitted, and Faulted	Inactive	Fault	Normal	Soak Test and Omitted	Inactive

Appendix D: AllowTamperMessages Config Entry

A new config key AllowTamperMessages is added to the Galaxy configuration file located in the path: Program Files (x86) \Tyco\CrossFire\ServerComponents.

Messages are filtered from the Zones based on the combination of Enabled check box (present on individual zone configuration window) and AllowTamperMessages config entry.

Figure 4: Config Key - AllowTamperMessages

```

TSP.Enterprise.Intrusion.Galaxy.Server.GalaxyDriverService.exe - Notepad
File Edit Format View Help
<?xml version="1.0"?>
<configuration>
  <appSettings>
    <add key="LaunchDebugger" value="0" />
    <add key="ClientSettingsProvider.ServiceUri" value="" />
    <add key="PanelSynchronizeBatchCount" value="3" />
    <add key="StatusPollInterval" value="800" />
    <add key="RetryCount" value="50" />
    <add key="RetryTimeout" value="10000" />
    <add key="CommandInterval" value="300" />
    <add key="ConnectionTimeout" value="60000" />
    <add key="AllowTamperMessages" value="0" />
    <add key="MaxInvalidAck" value="10" />
  </appSettings>

```

The following table lists the different combinations of Enabled check box and AllowTamperMessages config entry and the expected results.

Table 11: Different Combinations of Enabled Check Box and AllowTamperMessages Config Entry

S I. N o	Partitio n Status	AllowTamperMessag es config entry	Enable d check box	Result on generating Alarms (ShortCircuit, OpenCircuit, LowResistanc e, HighResistanc e, Masked, Faulted, ZoneMasked, ZoneFaulted, Tamper, Trouble, Alarm)	Results of clearing the alarm or tamper	Result on generating toggling (PIR) (Open /Open Loop/Close/Close d Loop)	Results on changen g the toggle switch
1	Set	1	Disable d	Alarm is reported in victor. All statuses (Alarm,	Closed and closed loop is	Alarm is reported in victor. All statuses (Alarm, Active, HW and Supervision) change in Dynamic	Closed and closed loop is

S I. N o	Partitio n Status	AllowTamperMessages config entry	Enable d check box	Result on generating Alarms (ShortCircuit, OpenCircuit, LowResistance, HighResistance, Masked, Faulted, ZoneMasked, ZoneFaulted, Tamper, Trouble, Alarm)	Results of clearing the alarm or tamper	Result on generating toggling (PIR) (Open /Open Loop/Close/Close d Loop)	Results on changen g the toggle switch
				Active, HW and Supervision) change in Dynamic View and are journaled in victor.	reported in victor. Alarm is then cleared in victor.	View and are journaled in victor.	reported in victor. Alarm is then cleared in victor.
2	Set	1	Enabled	Alarm is reported in victor. All statuses (Alarm, Active, HW and Supervision) change in Dynamic View and are journaled in victor.	Closed and closed loop is reported in victor. Alarm is then cleared in victor.	Alarm is reported in victor. All statuses (Alarm, Active, HW and Supervision) change in Dynamic View and are journaled in victor.	Closed and closed loop is reported in victor. Alarm is then cleared in victor.
3	Set	0	Disable d	No status update in Dynamic View. No journaling.	No status update in Dynamic View. No journaling.	No status update in Dynamic View. No journaling.	No status update in Dynamic View. No journaling.
4	Set	0	Enabled	Alarm is reported in victor. All statuses (Alarm, Active, HW and Supervision)	Closed and closed loop is reported in victor.	Alarm is reported in victor. All statuses (Alarm, Active, HW and Supervision) change in Dynamic View and are	Closed and closed loop is reported in victor.

S I. N o	Partitio n Status	AllowTamperMessag es config entry	Enable d check box	Result on generating Alarms (ShortCircuit, OpenCircuit, LowResistanc e, HighResistanc e, Masked, Faulted, ZoneMasked, ZoneFaulted, Tamper, Trouble, Alarm)	Results of clearing the alarm or tamper	Result on generating toggling (PIR) (Open /Open Loop/Close/Close d Loop)	Results on changen g the toggle switch
				change in Dynamic View and are journaled in victor.	Alarm is then cleared in victor.	journaled in victor.	Alarm is then cleared in victor.
5	Unset	1	Disable d	Alarm is reported in victor. All statuses (Alarm, Active, HW and Supervision) change in Dynamic View and are journaled in victor.	Closed and closed loop is reported in victor. Alarm is then cleared in victor.	No status update in Dynamic View. No journaling.	No status update in Dynamic View. No journalin g.
6	Unset	1	Enabled	Alarm is reported in victor. All statuses (Alarm, Active, HW and Supervision) change in Dynamic View and are journaled in victor.	Closed and closed loop is reported in victor. Alarm is then cleared in victor.	HW, Active, Supervision states change (Open, open loop, active) and journaled in victor. Alarm states do not change and are not journaled.	Closed and closed loop is reported in victor. Alarm is then cleared in victor.
7	Unset	0	Disable d	No status update in Dynamic View. No journaling.	No status update in Dynamic	No status update in Dynamic View. No journaling.	No status update in Dynamic

S I. N o	Partitio n Status	AllowTamperMessages config entry	Enable d check box	Result on generating Alarms (ShortCircuit, OpenCircuit, LowResistance, HighResistance, Masked, Faulted, ZoneMasked, ZoneFaulted, Tamper, Trouble, Alarm)	Results of clearing the alarm or tamper	Result on generating toggling (PIR) (Open /Open Loop/Close/Closed Loop)	Results on changing the toggle switch
					View. No journaling.		View. No journaling.
8	Unset	0	Enabled	Alarm is reported in victor. All statuses (Alarm, Active, HW and Supervision) change in Dynamic View and are journaled in victor.	Closed and closed loop is reported in victor. Alarm is then cleared in victor.	HW, Active, Supervision states change (Open, open loop, active) and journaled in victor. Alarm states do not change and are not journaled.	Closed and closed loop is reported in victor. Alarm is then cleared in victor.