



# Farrow Prescription Form

*Incomplete Forms Will Delay Shipping*

## Patient / Billing Information

Patient Name: \_\_\_\_\_ Prescriber: \_\_\_\_\_ UPIN: \_\_\_\_\_

Sex: M / F Age: \_\_\_\_\_ Height: \_\_\_\_\_ Weight: \_\_\_\_\_

Business: \_\_\_\_\_ Address: \_\_\_\_\_

City: \_\_\_\_\_ State: \_\_\_\_\_ Zip code: \_\_\_\_\_

Phone: \_\_\_\_\_ Fax: \_\_\_\_\_

Method of Payment: Check / Money Order \* Make checks payable to FarrowMed LLC \*

Credit Card (circle) -- Visa/MC/AMEX/Discover or PO # \_\_\_\_\_ Expires: \_\_\_\_\_

Signature of cardholder \_\_\_\_\_

## Shipping Information Same as above

Contact Person: \_\_\_\_\_ E-mail: \_\_\_\_\_

Business: \_\_\_\_\_ Address: \_\_\_\_\_


City: \_\_\_\_\_ State: \_\_\_\_\_ Zip code: \_\_\_\_\_

Phone: \_\_\_\_\_ Fax: \_\_\_\_\_

## Prescribing Information



	Left	Right
Thigh		
Leg		
Foot		
Toes		



Mild to Moderate Edema

Moderate to Severe Edema\*

\*Be cautious when prescribing "Moderate to Severe Edema" for patients with PAD.

If mixed severity, please specify in special instructions below.

	Left	Right
Arm		
Hand		
Fingers		



Special Instructions: \_\_\_\_\_

Related Diagnoses: \_\_\_\_\_

I authorize release of my name for identification purposes.

### Prescriber

\_\_\_\_\_  
Patient Name (please print)      Signature

\_\_\_\_\_  
Selection Permitted

\_\_\_\_\_  
Dispense as written

\_\_\_\_\_  
Date

\_\_\_\_\_  
Date


Refill: \_\_\_\_\_ times PRN NR

FarrowMed LLC  
 Ph: (979) 822-9120 • Fax: (979) 775-5202  
 www.FarrowMed.com

Input your institution's contact information here

# Farrow Microfine and FarrowWrap® Gauntlet Order Form

Business: \_\_\_\_\_ Patient: \_\_\_\_\_ PO: \_\_\_\_\_  
 Person Measuring: \_\_\_\_\_ Phone/Fax: \_\_\_\_\_ / \_\_\_\_\_ Date: \_\_\_\_\_

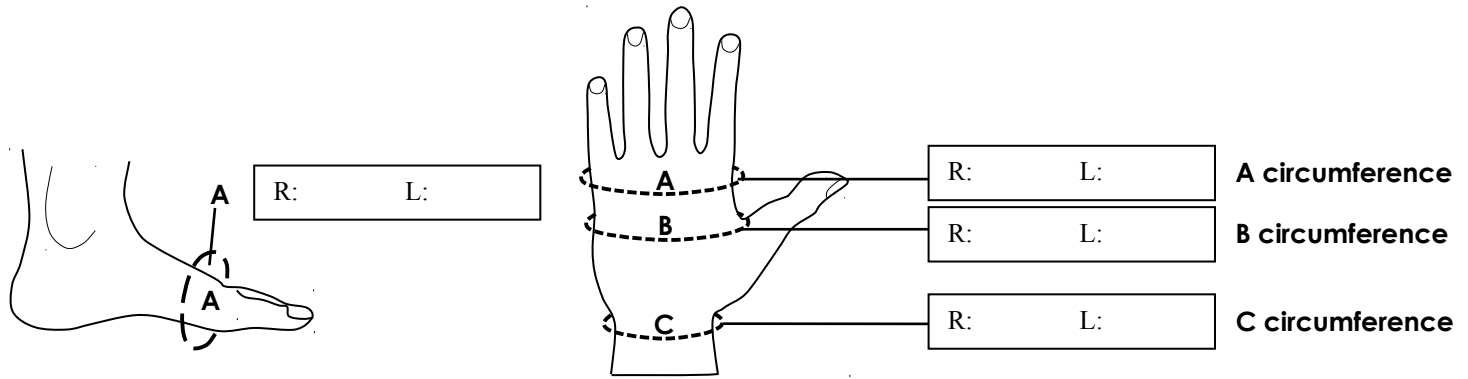

Farrow Microfine Gloves and Toe Caps provide Class I compression and are ambidextrous. The fingers and toes of the garments can be trimmed using normal scissors and won't fray or roll.

FarrowWrap LITE™ Hand Gauntlet is ambidextrous and can be worn with FarrowFoam™ squares (one 4mm & one 8mm), which are ordered separately. They are suitable for mild to severe edemas. The gauntlet can be worn by itself or over a Microfine glove, for extra dorsal hand compression.

Microfine Class I Glove		XSmall	Small	Medium	Large
(A) Base of Fingers		16 – 18 cm	18 – 20 cm	20 – 22 cm	22 – 24 cm
(B) Fold of Thumb		17 – 19 cm	19 – 21 cm	21 – 23 cm	23 – 26 cm
(C) Wrist		15 – 18 cm	17 – 20 cm	19 – 22 cm	22 – 24 cm
<b>Microfine Glove - ½ Finger Length - Black</b>	FSMF-T-HHB	Qty	Qty	Qty	Qty
<b>Microfine Glove - ½ Finger Length - Copper</b>	FSMF-T-HHC	Qty	Qty	Qty	Qty
<b>Microfine Glove - ½ Finger Length - Sand</b>	FSMF-T-HHS	Qty	Qty	Qty	Qty
<b>Microfine Glove - Full Finger Length - Black</b>	FSMF-T-HFB	Qty	Qty	Qty	Qty
<b>Microfine Glove - Full Finger Length - Copper</b>	FSMF-T-HFC	Qty	Qty	Qty	Qty
<b>Microfine Glove - Full Finger Length - Sand</b>	FSMF-T-HFS	Qty	Qty	Qty	Qty
FarrowWrap® Hand Gauntlet		XSmall	Small	Medium	Large
<b>LITE Ambidextrous Hand Gauntlet</b>	FWLT-O-HGAT	Qty	Qty	Qty	Qty
<b>Gauntlet Foam &amp; Velcro Replacement Pack</b>	FWLT-O-HGRP	Qty		Qty	

Microfine Class I Toe Cap		XSmall	Small	Medium	Large
(A) Base of Toes		21 – 23 cm	23 – 25 cm	25 – 27 cm	27 – 29 cm
<b>Microfine Toe Cap – Black</b>	FSMF-T-MB	Qty	Qty	Qty	Qty
<b>Microfine Toe Cap – Copper</b>	FSMF-T-MC	Qty	Qty	Qty	Qty
<b>Microfine Toe Cap – Sand</b>	FSMF-T-MS	Qty	Qty	Qty	Qty

## Directions for Glove, Gauntlet, and Toe Cap

Fill in the Patient / Billing & Shipping Information areas **completely**. Measure hand and/or foot circumferences at specified areas and mark on form. Cross reference measurements with measurements on form's chart to determine the correct size garment. In the blank white box indicate the number of garments desired. Microfine and FarrowWrap® Hand Gauntlets are sold as eaches.

The associated SKU number can be cross-referenced with the Pricing Schedule to calculate the price. A practitioner's order is required for all garments. DME stores do not need to forward a practitioner's order to FarrowMed. Have the patient sign the authorization.

### Microfine

#### Microfine Glove Measuring Instructions

Measure hand at base of fingers, fold of thumb, and wrist. Match measurements to appropriate sized glove. If the measurements do not match, stop here. This glove will not fit.

#### Trimming and Fitting Instructions

1. Apply appropriate sized glove.
2. If the glove fingers are too long, with a pencil mark the point along the glove fingers at which they should be trimmed.
3. Remove glove.
4. Trim the glove fingers at all points marked with pencil; then, reapply the glove.
5. Do not trim while patient has glove donned.

#### Microfine Toe Cap Measuring Instructions

Measure base of toes and match measurements to appropriate sized Toe Cap. If the measurement does not match, stop here. This Toe Cap will not fit.

#### Trimming and Fitting Instructions

1. Apply appropriate sized toe cap.
2. If the toe cap toes are too long, place a mark the point along the toe cap toes at which they should be trimmed with a pencil.
3. Remove toe cap.
4. Trim the toe cap toes at all points marked with pencil; then, reapply the toe cap.
5. Do not trim while patient has garments donned.

### Gauntlet

#### FarrowWrap® Hand Gauntlet Measuring Instructions

Measure hand at base of fingers, fold of thumb, and wrist. Match measurements to the appropriate sized gauntlet. If the measurements do not match, stop here. This gauntlet will not fit.

If the gauntlet thumbhole is too small, it can be trimmed larger by a fitter, but **exercise caution not to cut off too much fabric or cut across seams**. If the thumb swells, a glove will be needed to control the swelling.

#### Fitting Instructions

1. Place the gauntlet on a table in front of you. The thumbhole should be closer to the center of the body for the hand on which it will be placed, with the thinner band further away from you.
2. To attach foam, flip the gauntlet over and attach either the 4 or 8 mm foam using the Velcro® tabs on the foam about 1 cm from the thumbhole.
3. Attach the Velcro® pieces to the appropriate bands on the side opposite the foam leaving about half sticking off the edge.

