



GroStar[®]

AI103G

GS3 Premium EC/ppm Pen
(Gen II)

User Guide

Scan to watch the video tutorial



Contents

	page
01 Main Features	2
02 Preparation Before First Use	3
03 EC Calibration	4
04 EC/500ppm/700ppm Measurement	5
05 Other Functions	5
5.1 Reading Hold	5
5.2 Temperature Unit Switch	5
5.3 TruRead Measurement Mode	5
5.4 Auto. Power Off	5
06 Probe Cleaning	6
07 Probe Storage	6
08 Battery Replacement	7
09 Probe Replacement	7
10 Notes	7
11 Troubleshooting Guide	8
12 Technical Specs	9
13 Accessories	10
14 Limited Warranty	

Thank you for choosing the GroStar® GS3 Premium EC/ppm Pen (gen II). This premium pen has been designed specifically for the horticultural market. Since 1991, Apera instruments has been dedicated to providing advanced lab-grade instruments and sensors. GroStar's intelligent design reduces the guesswork so you can easily manage your crops success.

01 Main Features

- Premium titanium alloy conductivity probe measures EC, ppm (500/700) all-in-one unit with minimal maintenance.
- Easy-to-use design and quick 1-point calibration adjustment.
- 3-Color backlit LCD screen gives you clear readings in different modes even in dark environment.
- Durable structure, IP67 waterproof rating, powered by AAA batteries.
- The probe is replaceable, so you don't have to discard the entire pen when the probe reaches its end of life.

Color LCD Screen

- White for measurement mode
- Green for calibration mode
- Red for calibration error

M stands for stabilized reading

M stands for successful calibration: M is 2.77 EC. The icon disappears in 30 days to remind you for re-calibration.

Probe Cap

- Water droplets are added during production to maintain the moisture of the probe. This is a normal practice and should not be attributed to used product.
- The Fill line shows the level to which you should pour the soaking solution or sample solution.
- For details of probe storage, see Section 7.


	Short Press	Long Press
	1. Power on 2. Manual hold Press again to cancel hold.	Power off
	In measurement mode, press to enter TruRead mode	Start calibration
	Switch mode: EC→500ppm→700ppm	Switch between °F and °C

Premium Conductivity Probe


- The titanium alloy conductivity sensor is highly accurate and requires minimal maintenance.
- The probe is replaceable, saving money in the long run.

02 Preparation Before First Use

2.1 Pull out the battery insulation slip, and take off the probe cap.

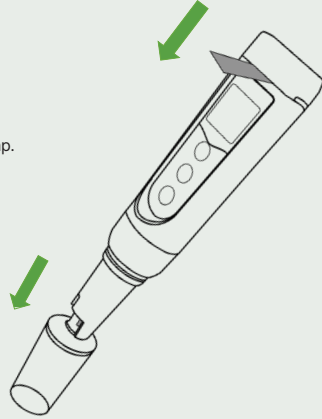


2.2 Rinse the probe with clean water, then shake off excess water.

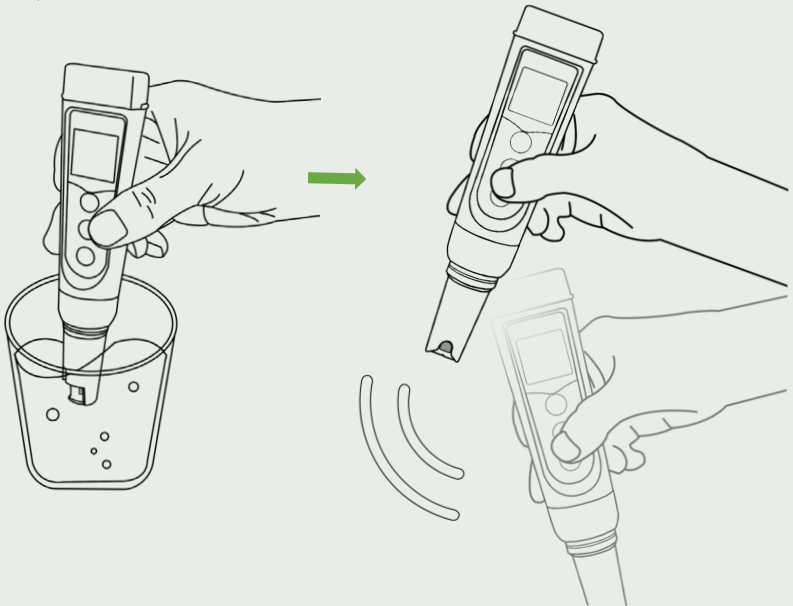


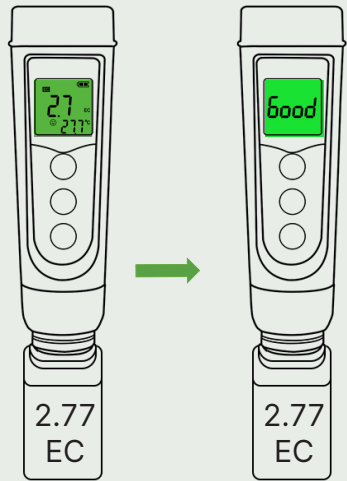
2.3 Calibrate EC at 2.77 EC standard solution. For calibration tutorial, see Section 3.



03 EC Calibration


3.1 Power on and remove the probe cap. Rinse the probe with clean water and shake-dry, then submerge it in the 2.77 EC standard solution; **shake the probe vertically in the solution bottle for a few seconds**, then let it stand.

3.2 Hold  until screen turns green. The tester starts the automatic calibration. Wait for "Good" to show up (in 10-15 seconds), indicating the calibration is completed, then the tester returns to measurement mode.


 Short press any key while calibrating (in green screen) to cancel calibration and return to measurement.



3.3  icon will show up on the lower left corner indicating a successful calibration.  disappears in 30 days after calibration, reminding you to re-calibrate EC. We recommend calibrating the EC once every month to ensure accuracy. If you feel like the accuracy might be off, simply test the standard solution (make sure the solution is fresh and clean). If the reading is greater than 2.8 EC or smaller than 2.7 EC, it's time to calibrate again.




3.4 If the calibration fails, the screen will turn red. For details, see Section 11 Troubleshooting Guide.



04 EC/500ppm/700ppm Measurement

- 4.1 Power on and remove the probe cap.
- 4.2 Rinse the probe with clean water and shake off excess water.
- 4.3 Submerge the probe into the solution, make a quick stir in the solution. Hold still and wait for the reading to stabilize (☺ stays on the screen), then record the reading.
- 4.4 Short press to switch from EC → 500ppm → 700ppm
- 4.5 Thoroughly rinse the probe with clean water, then put on the probe cap.

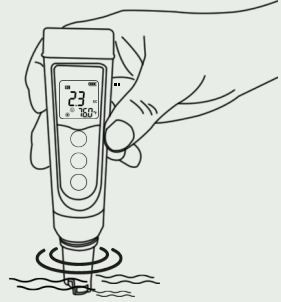

What is EC and its relation to 500ppm & 700ppm?

EC (electrical conductivity) is a measure of the nutrients in the solution. Low EC indicates a low nutrient concentration, which usually results in nutritional deficiencies and slow growth rates of plants. A higher conductivity indicates more food for plants. However, be careful with abnormally high levels. Delicate plants, cuttings, and seedlings can experience fertilizer burn if the conductivity is excessively high.

EC, 500ppm, and 700ppm are simply different units preferred by different markets. 500ppm and 700ppm both originate from EC. Therefore, using EC to compare and analyze test results is the safest way and minimizes confusion. Here is how they convert to each other:

- 1.0 (EC) = 500ppm (500ppm) = 700ppm (700ppm)
 2.6 (EC) = 1300ppm (500ppm) = 1820ppm (700ppm)




05 Other Functions

- 5.1 If needed, you can manually hold (lock) the reading by short pressing . Press it again to cancel the hold.
- 5.2 Long press to switch temp. units between °F and °C.
- 5.3 Short press to enter **TruRead** mode. As you perform testing, the pen automatically records measurements after each reading is stabilized for 7 seconds ("01" will show up at the bottom right to indicate the 1st set of data is recorded). After you finish all the testing, short press again to check the average, maximum, and minimum values of all the recorded measurements. Then short press again to end TruRead mode and return to normal measurement mode.
- 5.4 The tester will automatically power off if there is no operation within 10 minutes. If you want to turn off the Auto. Power Off function, power off the tester, and then hold for 5 seconds until you see Auto off. Then it will power on and go to measurement mode automatically.



06 Probe Cleaning

6.1 The tester is only accurate the probe is clean. Always thoroughly rinse the probe before and after each measurement with clean water in a container or with a wash bottle.

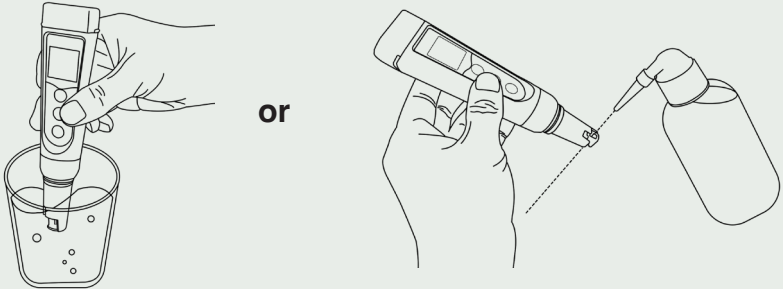


6.2 For tough contaminants, soak the probe in Apera's cleaning solution or detergent water for 30 minutes. Then use a soft brush to remove the contaminants. Afterwards, rinse it off, then re-calibrate the tester before using it again. These cleaning tools can be found in Apera's Probe Care Kit (see Section 13).


07 Probe Storage

7.1 Under regular usage (daily or weekly use), just make sure probe cap is wet, and tightened with the red O-ring.

7.2 For long-term storage (you are not going to use the product for more than a month), add clean water to the Fill line in the probe cap and store the probe in it. Cover on the probe cap tightly.

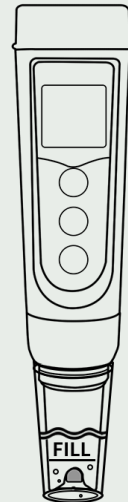


08 Battery Replacement

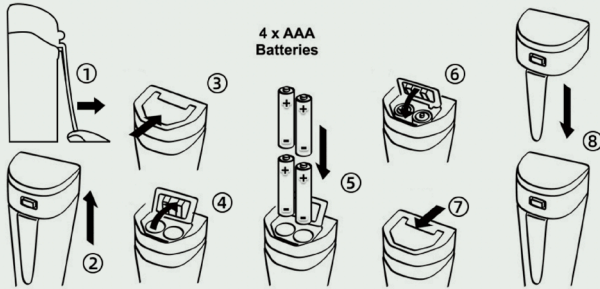

- ① Loosen the battery cap lock.
- ② Pull off the battery cap.
- ③ Slide the battery cover along the OPEN arrow to open the cover.
- ④ Open the battery cover.
- ⑤ Insert the batteries (**ALL POSITIVE SIDES FACING UP**).
- ⑥ Press down the battery cover and hold it.
- ⑦ Slide the battery cover along the LOCK arrow to lock the cover.
- ⑧ Close the battery cap. Make sure to push it all the way down.

The tester's waterproof rating may be compromised if the battery cap is not tightly closed.

09 Probe Replacement



Twist off the probe ring, unplug the old probe; plug in the new probe (make sure to align the connector's position properly), and twist on the probe ring.



Probes don't last forever. Every probe will eventually age and fail even if you don't use it that often. The typical service life of GroStar probes is 18-24 months depending on the frequency of usage and how well you keep it clean and properly stored.

We recommend replacing your EC probe at least every 18 months to ensure the best accuracy.


The nice thing about GroStar pens is that you can just buy a replacement probe instead of a whole new tester.

10 Notes


- 10.1 Avoid testing in high (>113°F) or low temperature (<41°F) solutions as it will cause greater measurement error and damage to the probe. Test your samples and perform calibration close to room temperature as much as possible.
- 10.2 Make sure the battery cap is completely tightened with the O-ring. Otherwise, the waterproof rating could be compromised.

11 Troubleshooting Guide

Trouble	Reason	How to fix
 Cannot calibrate	Poor quality standard solutions	Replace with fresh and clean standard calibration solutions made by legitimate manufacturers.
	Contaminated probe	Clean the probe with Apera's cleaning solution or detergent water.
	Aged probe	Replace the probe.
	Dried-out probe	Soak the probe in clean water for 30 minutes.
	Probe is not fully submerged in the solution	Make sure the probe is fully immersed in the solution at least 1 inch deep.
Reading is always slowly changing, won't stabilize.	Contaminated probe	Clean the probe with Apera's cleaning solution or detergent water.
	Aged probe	Replace the probe.
Display similar readings in any solutions	Broken probe	If you don't find any visible damage of the probe and it's within the 1-year probe warranty, contact your point of purchase for warranty fulfillment; If there is visible damage or the probe is aged, replace the probe.
Reading keeps jumping	Probe is not fully submerged in the solution	Make sure the probe is fully immersed in the solution at least 1 inch deep.
	Air bubbles around the sensor	Make a quick stir in the solution to remove air bubbles.
	Probe is not properly connected or the pin connector is broken.	Check the probe's connector, make sure it's not broken and is connected. Align the probe and instrument correctly before plugging in. Never force it. Ensure the probe connector is not exposed in the air too long.
Calibration is successful, but reading is not accurate	Aged probe	Replace the probe.
	Air bubbles around the sensor	Make a quick stir in the solution to remove air bubbles.
	Comparison with other testers	To compare with other testers, make sure to perform calibration for all testers in the same standard, then test another standard (e.g. Apera's 1413µS=1.4 EC). Whichever gives more accurate reading in the other standard is the more accurate one.





Out of range reminder for EC



Out of range reminder for temperature

12 Technical Specs

Range	0.0-10.0 EC, 0-7000ppm (700ppm), 0-5000ppm (500ppm), 0-50°C (32-122 °F)
Resolution	0.1 EC, 10 ppm (700ppm), 10ppm (500ppm), 0.1°C /0.1 °F
Accuracy	±0.1 EC, ±30 ppm (500ppm) ±40ppm (700ppm) ±1°C /±1 °F
Temperature compensation	Automatic
Calibration	Automatic 1 point (2.77 EC)
Unit	EC, 500ppm, 700ppm, °C , °F
Power supply	4-AAA alkaline batteries
Backlight	White (measurement) ; Green (calibration) ; Red (error)
Reading hold	Manual
Warranty	Two years for the instrument, one year for the probe
EC probe	Titanium alloy
Successful calibration indicator	M (2.77 EC)
Low battery reminder	
Waterproof rating	IP67
Reading stabilization icon	

What's in the box?



13

Accessories

Probe Care Accessories

Probe Cleaning Solution
SKU: AI1166



CalPod Solution Organizer
SKU: AI2910



Probe Cleaning Brush
SKU: AI2915



Replacement Probe

GS3-E
EC Probe



2.77 EC Calibration Solution



How Long Does the Coverage Last?

Apera Instruments® (Apera) warrants the GroStar® GS3 EC/ppm Pen Tester (Product) for a period of 24 months for the instrument and 12 months for the probe from date of purchase by original purchaser or consumer. Proof of purchase is required for the warranty to be effective (store sales receipt for Product showing model number, payment and date of purchase). This warranty is non-transferable and terminates if the original purchaser/consumer sells or transfers the Product to a third party.

What is Covered?

Apera warrants the Product against defects in material and workmanship when used in a normal manner, in accordance with Apera instruction manuals. If Apera is provided with valid proof of purchase (as defined above) and determines the Product is defective, Apera may, in its sole discretion either (a) repair the Product with new or refurbished parts, or (b) replace the Product with a new or refurbished Product.

What is NOT Covered?

This warranty does not apply to any equipment, component or part that was not manufactured or sold by Apera, and shall be void if any such item is installed on a Product. Further, this warranty does not apply to replacement of items subject to normal use, wear and tear and expressly excludes:

- Cosmetic damage such as stains, scratches and dents
- Damage due to accident, improper use, negligence, careless operation or handling of Product not in accordance with Apera instruction manuals, or failure to maintain or care for Product as recommended by Apera
- Damage caused by use of parts not assembled/installed per Apera instructions
- Damage caused by use of parts or accessories not produced or recommended by Apera
- Damage due to transportation or shipment of Product
- Product repaired or altered by parties other than Apera or its authorized agents
- Product with defaced, missing or illegible serial numbers
- Products not purchased from Apera or an Apera-authorized distributor or reseller.

Limitation of Liability & Acknowledgments

TO THE MAXIMUM EXTENT PERMITTED BY LAW, THIS WARRANTY AND THE REMEDIES SET OUT ABOVE ARE EXCLUSIVE AND IN LIEU OF ALL OTHER WARRANTIES, GUARANTEES AND REMEDIES (ORAL OR WRITTEN, EXPRESS OR IMPLIED). EXCEPT AS PROVIDED IN THIS WARRANTY AND TO THE MAXIMUM EXTENT PERMITTED BY LAW, APERA INSTRUMENTS IS NOT RESPONSIBLE FOR SPECIAL, INCIDENTAL OR CONSEQUENTIAL LOSS OR DAMAGES, OR ANY OTHER LOSS OR DAMAGES RESULTING FROM SALE OR USE OF THE PRODUCT, OR BREACH OF WARRANTY, HOWEVER CAUSED, INCLUDING DAMAGES FOR LOST PROFITS, PERSONAL INJURY OR PROPERTY DAMAGE.

IT IS UNDERSTOOD AND AGREED BY CONSUMER UPON PURCHASE OF A PRODUCT THAT, EXCEPT AS STATED IN THIS WARRANTY, APERA INSTRUMENTS IS NOT MAKING AND HAS NOT MADE ANY EXPRESS OR IMPLIED WARRANTY OR OTHER REPRESENTATION REGARDING THE PRODUCT, AND DISCLAIMS ANY WARRANTY OF MERCHANTABILITY OR FITNESS FOR A PARTICULAR PURPOSE TO THE EXTENT PERMITTED BY LAW. ANY WARRANTIES WHICH ARE IMPOSED BY LAW AND CANNOT BE DISCLAIMED ARE HEREBY LIMITED IN DURATION TO THE PERIOD AND REMEDIES PROVIDED IN THIS WARRANTY.

SOME JURISDICTIONS (STATES OR COUNTRIES) DO NOT ALLOW EXCLUSION OR LIMITATION FOR INCIDENTAL OR CONSEQUENTIAL DAMAGES, OR LIMITATION ON HOW LONG AN IMPLIED WARRANTY LASTS, SO THE ABOVE LIMITATION OR EXCLUSION MAY NOT BE APPLICABLE. IF ANY PROVISION OF THIS WARRANTY IS JUDGED TO BE ILLEGAL, INVALID OR UNENFORCEABLE, THE REMAINING PROVISIONS OF THE WARRANTY SHALL REMAIN IN FULL FORCE AND EFFECT.

Governing Law; Authority

This warranty is governed by the laws of the state of country where Product is purchased, without regard to its choice of law principles. Except as allowed by law, Apera does not limit or exclude other rights a consumer may have with regard to the Product. No Apera distributor, employee or agent is authorized to modify, extend or otherwise change the terms of this warranty.



Address: 6656 Busch Blvd, Columbus Ohio 43229

Tel: 1-614-285-3080

Email: info@aperainst.com

Website: aperainst.com